

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027581.D
 Acq On : 30 Aug 2022 13:11
 Operator : SY/MD
 Sample : N4402-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	67539	79526	16.06%	2.020%
2	1.452	122	128	134	rBV3	8109	8872	1.79%	0.225%
3	1.564	156	163	176	rVB	60803	71435	14.42%	1.814%
4	2.105	321	331	344	rVV	127886	185971	37.55%	4.723%
5	2.166	345	350	367	rVB9	6386	14327	2.89%	0.364%
6	2.506	446	456	466	rBV4	4414	7285	1.47%	0.185%
7	2.770	533	538	550	rVB4	4481	7575	1.53%	0.192%
8	3.892	877	887	911	rBV2	43031	140888	28.45%	3.578%
9	4.346	1014	1028	1050	rBV	89699	233136	47.07%	5.921%
10	5.043	1231	1245	1280	rBV2	184024	495279	100.00%	12.579%
11	5.616	1411	1423	1460	rBV	165652	373536	75.42%	9.487%
12	5.921	1505	1518	1530	rBV	6462	15703	3.17%	0.399%
13	6.069	1547	1564	1597	rBV2	114563	255060	51.50%	6.478%
14	6.989	1839	1850	1871	rBV	37743	80108	16.17%	2.035%
15	7.317	1938	1952	1974	rBV	182138	338529	68.35%	8.598%
16	7.628	2038	2049	2065	rBV	22847	45821	9.25%	1.164%
17	8.091	2178	2193	2226	rBV	170294	376646	76.05%	9.566%
18	8.850	2418	2429	2452	rBV	255423	431542	87.13%	10.961%
19	10.217	2843	2854	2869	rBV	75416	118738	23.97%	3.016%
20	11.249	3162	3175	3192	rBV	220719	353596	71.39%	8.981%
21	11.535	3250	3264	3273	rBV3	15814	30734	6.21%	0.781%
22	11.622	3280	3291	3314	rVB	168658	272906	55.10%	6.931%




Sum of corrected areas: 3937213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027581.D
Acq On : 30 Aug 2022 13:11
Operator : SY/MD
Sample : N4402-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

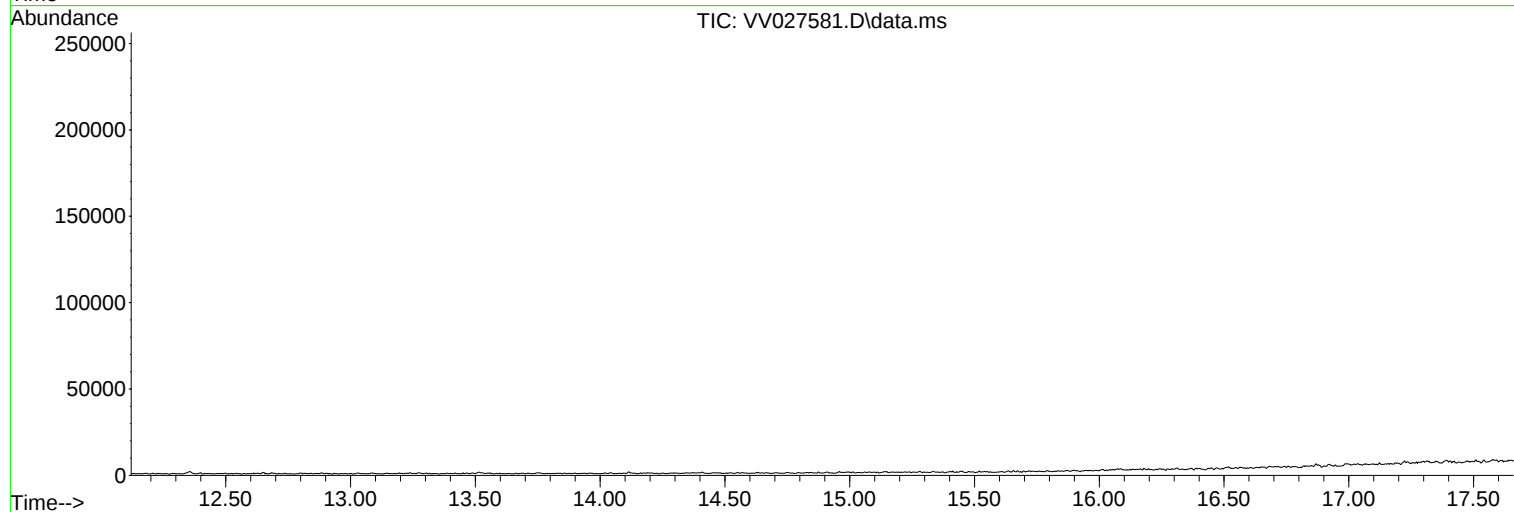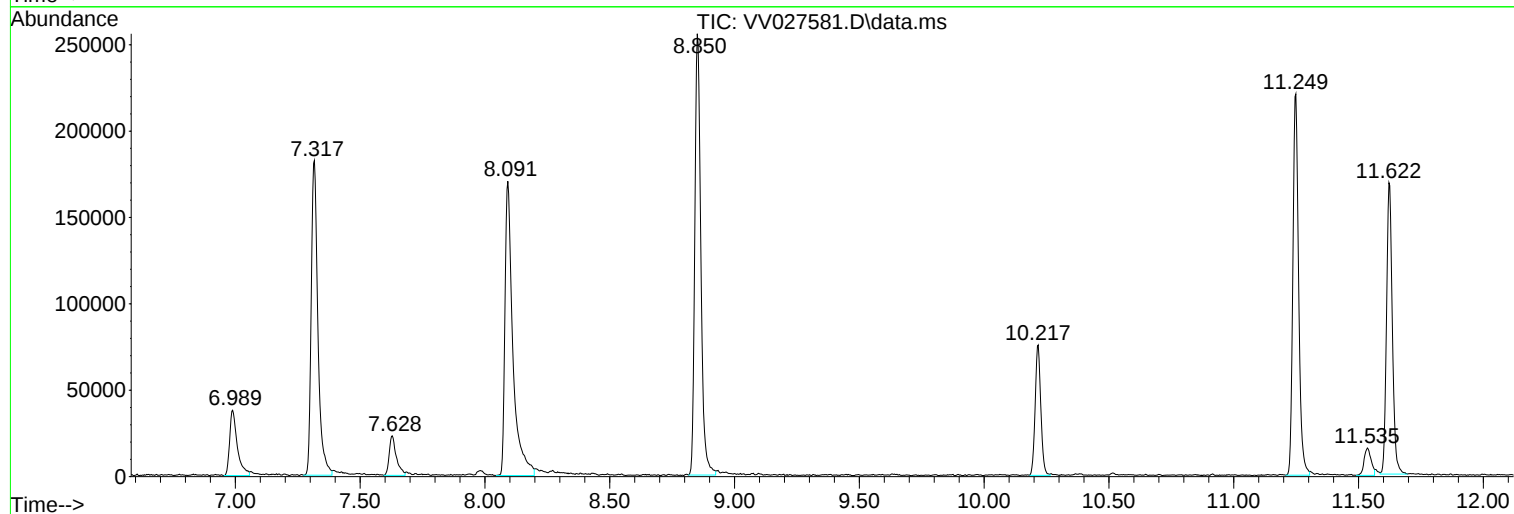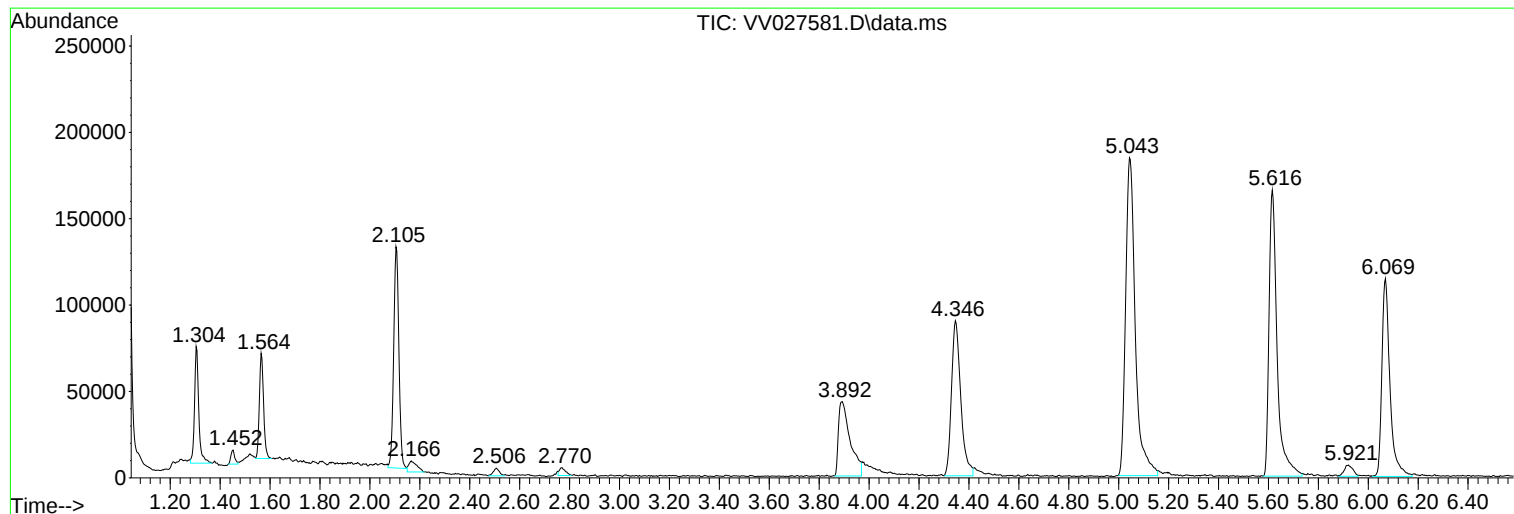

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027581.D
Acq On : 30 Aug 2022 13:11
Operator : SY/MD
Sample : N4402-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027581.D
Acq On : 30 Aug 2022 13:11
Operator : SY/MD
Sample : N4402-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc