

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027584.D
 Acq On : 30 Aug 2022 14:24
 Operator : SY/MD
 Sample : N4368-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	30	rVB3	4989	6209	1.16%	0.150%
2	1.304	70	82	92	rBV	73897	89464	16.73%	2.166%
3	1.564	157	163	177	rBV	63636	78993	14.78%	1.913%
4	2.105	322	331	345	rVB	134131	195970	36.66%	4.745%
5	3.175	652	664	678	rBV3	7438	17365	3.25%	0.420%
6	3.761	833	846	860	rBV7	5344	14121	2.64%	0.342%
7	3.899	880	889	911	rBV	31848	108528	20.30%	2.628%
8	4.349	1011	1029	1046	rBV2	93134	235618	44.07%	5.705%
9	4.670	1116	1129	1130	rBV6	20106	25253	4.72%	0.611%
10	5.047	1229	1246	1290	rBV2	198350	534631	100.00%	12.945%
11	5.616	1407	1423	1454	rBV	170071	379793	71.04%	9.196%
12	6.069	1550	1564	1593	rBV	120304	268934	50.30%	6.512%
13	6.989	1840	1850	1870	rBV	43198	92802	17.36%	2.247%
14	7.317	1940	1952	1976	rBV	192032	361995	67.71%	8.765%
15	7.625	2040	2048	2066	rBV	24926	49334	9.23%	1.195%
16	8.092	2183	2193	2235	rBV	167550	416925	77.98%	10.095%
17	8.850	2419	2429	2453	rBV	268665	459090	85.87%	11.116%
18	10.217	2842	2854	2866	rBV	81309	132226	24.73%	3.202%
19	11.249	3163	3175	3190	rBV	229139	364301	68.14%	8.821%
20	11.622	3280	3291	3307	rBV	172931	282194	52.78%	6.833%
21	16.178	4701	4708	4716	rVB10	6889	10435	1.95%	0.253%
22	16.705	4867	4872	4881	rVB8	4383	5898	1.10%	0.143%


Sum of corrected areas: 4130079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027584.D
Acq On : 30 Aug 2022 14:24
Operator : SY/MD
Sample : N4368-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

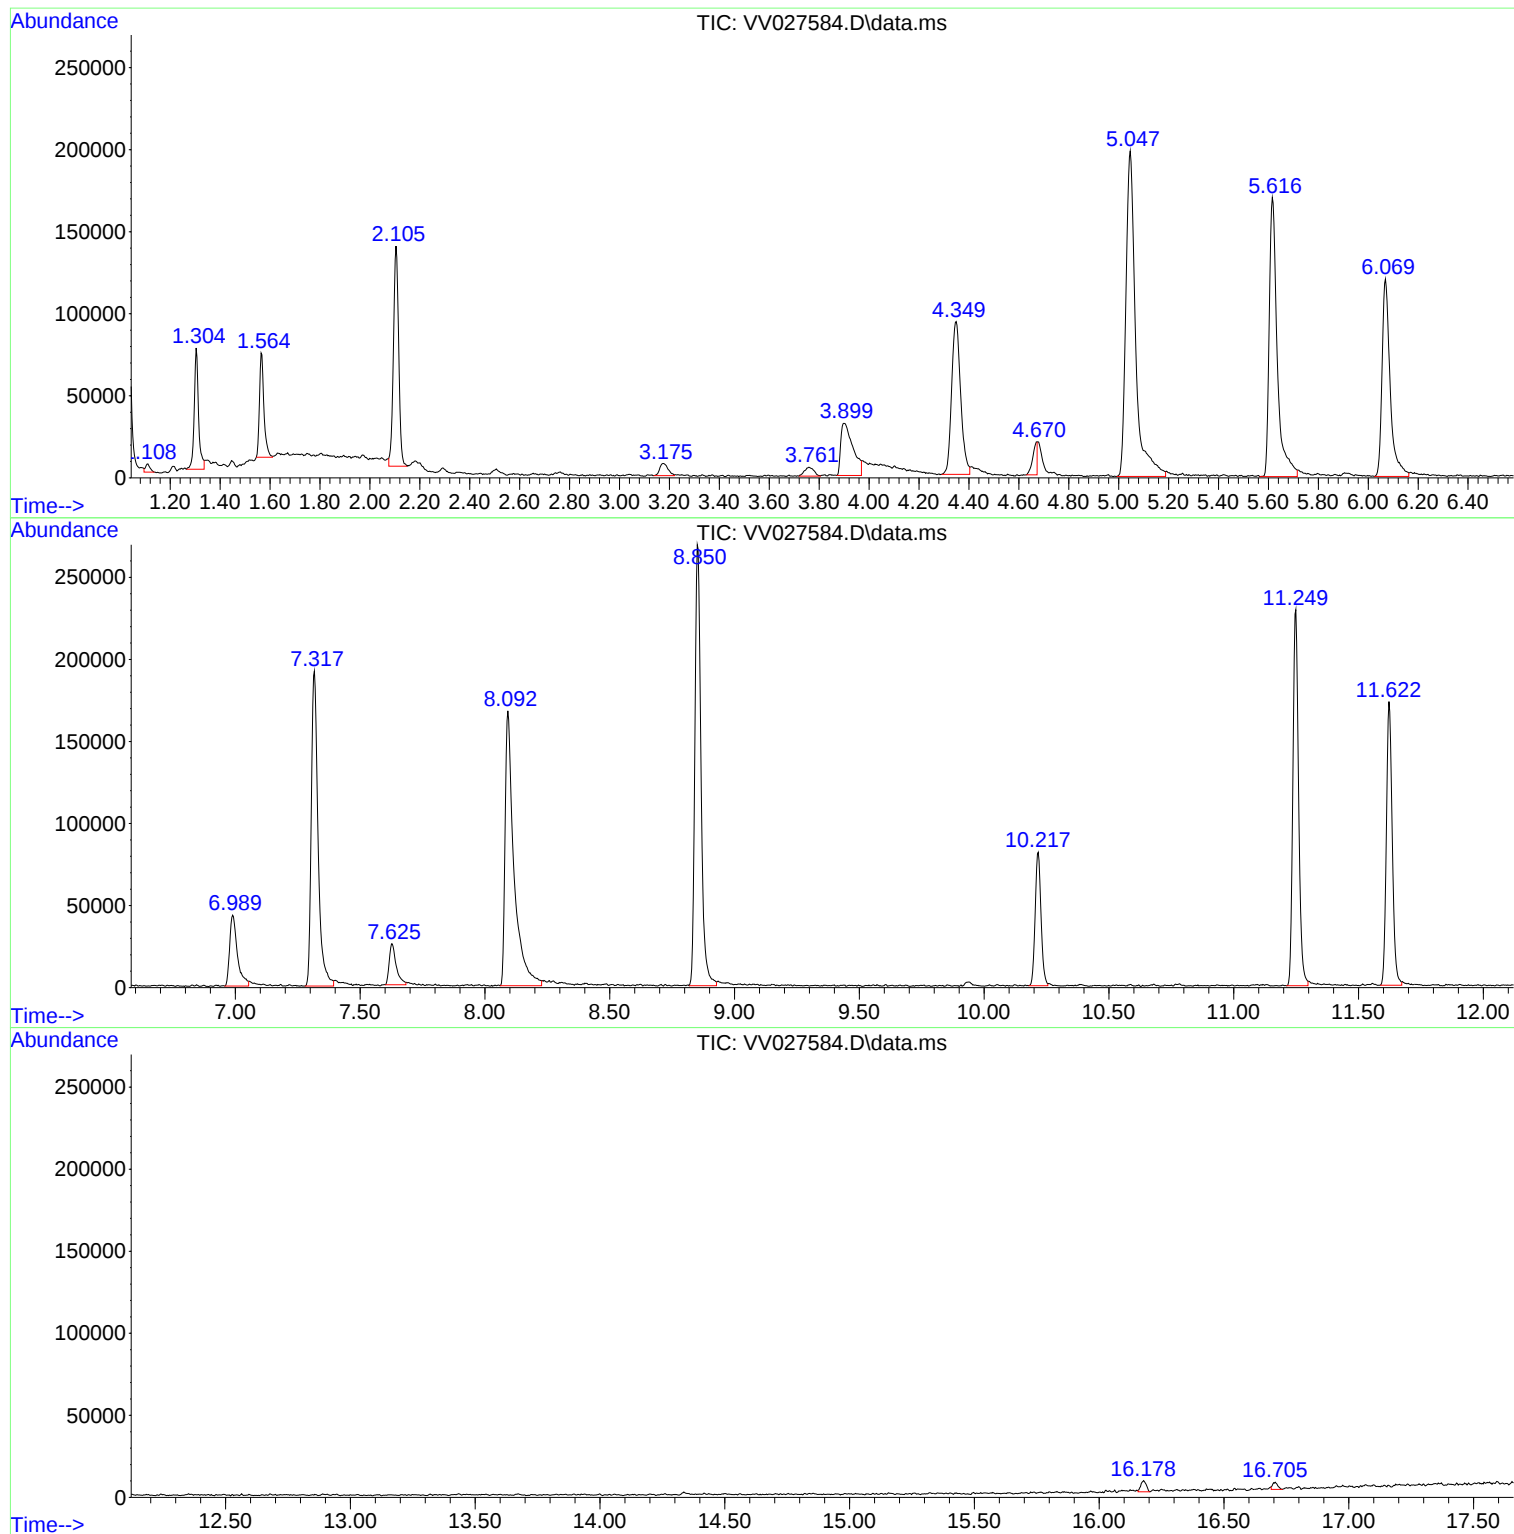

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027584.D
Acq On : 30 Aug 2022 14:24
Operator : SY/MD
Sample : N4368-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027584.D
Acq On : 30 Aug 2022 14:24
Operator : SY/MD
Sample : N4368-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc