

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027589.D
 Acq On : 30 Aug 2022 16:27
 Operator : SY/MD
 Sample : N4404-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVC4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	64317	71580	14.95%	1.823%
2	1.452	123	128	132	rBV4	6102	6586	1.38%	0.168%
3	1.564	157	163	175	rVB	59823	69688	14.55%	1.775%
4	2.105	320	331	344	rBV	128550	184926	38.62%	4.711%
5	2.182	346	355	373	rVB6	9744	27637	5.77%	0.704%
6	3.892	877	887	905	rBV	46415	135610	28.32%	3.455%
7	4.346	1011	1028	1064	rBV	91100	244019	50.96%	6.216%
8	5.047	1227	1246	1265	rBV3	187829	478848	100.00%	12.199%
9	5.616	1410	1423	1454	rBV	163382	364394	76.10%	9.283%
10	6.069	1550	1564	1593	rBV	114712	252185	52.66%	6.424%
11	6.989	1838	1850	1871	rBV2	37005	75676	15.80%	1.928%
12	7.317	1939	1952	1975	rBV	187922	341372	71.29%	8.696%
13	7.629	2040	2049	2063	rBV3	21988	44608	9.32%	1.136%
14	7.982	2151	2159	2166	rBV9	3587	5881	1.23%	0.150%
15	8.092	2183	2193	2226	rBV	178546	386047	80.62%	9.834%
16	8.850	2418	2429	2452	rBV	259469	444005	92.72%	11.311%
17	10.214	2842	2853	2870	rBV	75814	122920	25.67%	3.131%
18	11.249	3163	3175	3194	rBV	222765	353306	73.78%	9.000%
19	11.532	3253	3263	3275	rBV2	22690	42877	8.95%	1.092%
20	11.622	3281	3291	3306	rBV	170529	273279	57.07%	6.962%




Sum of corrected areas: 3925444

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027589.D
Acq On : 30 Aug 2022 16:27
Operator : SY/MD
Sample : N4404-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

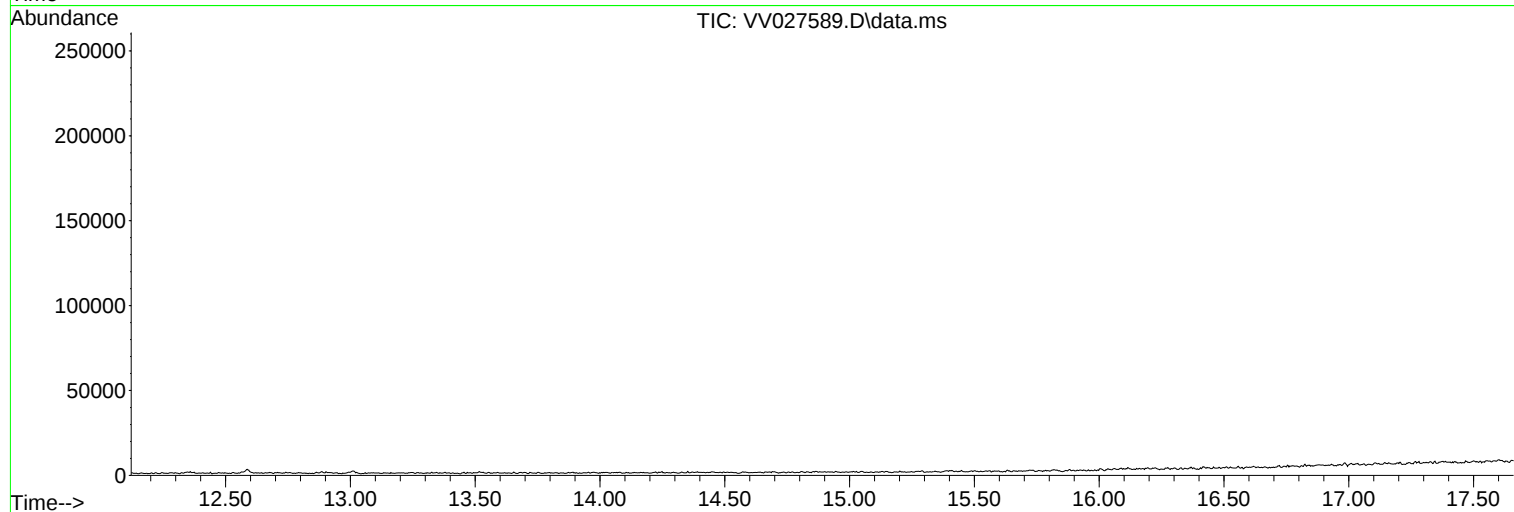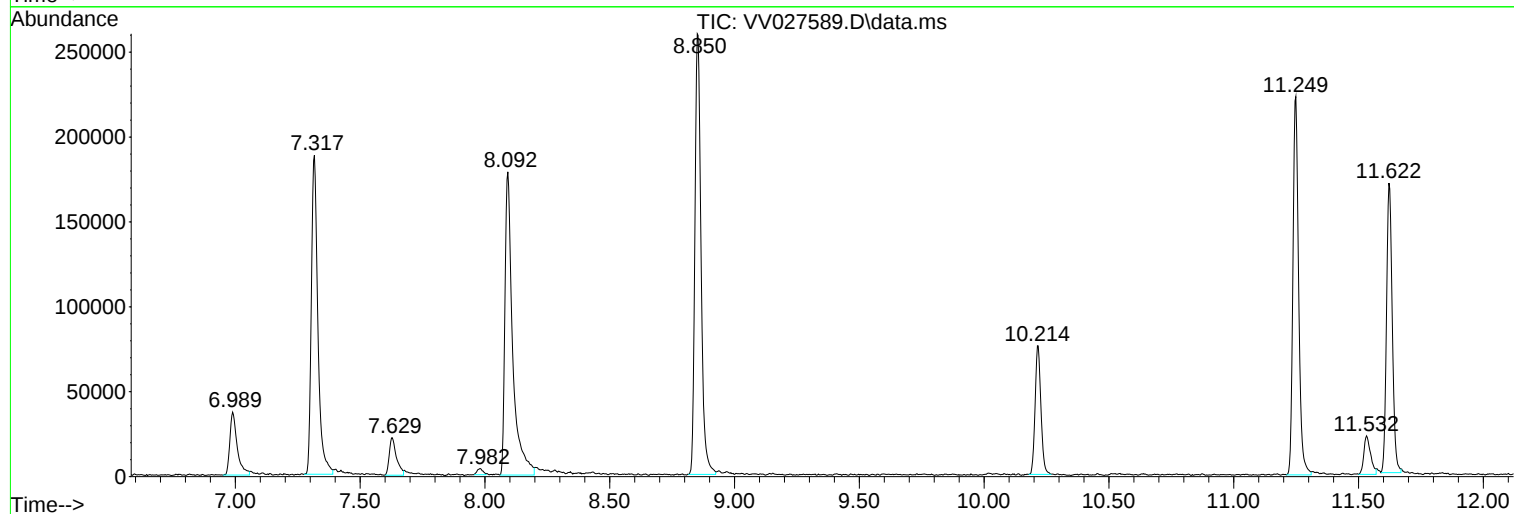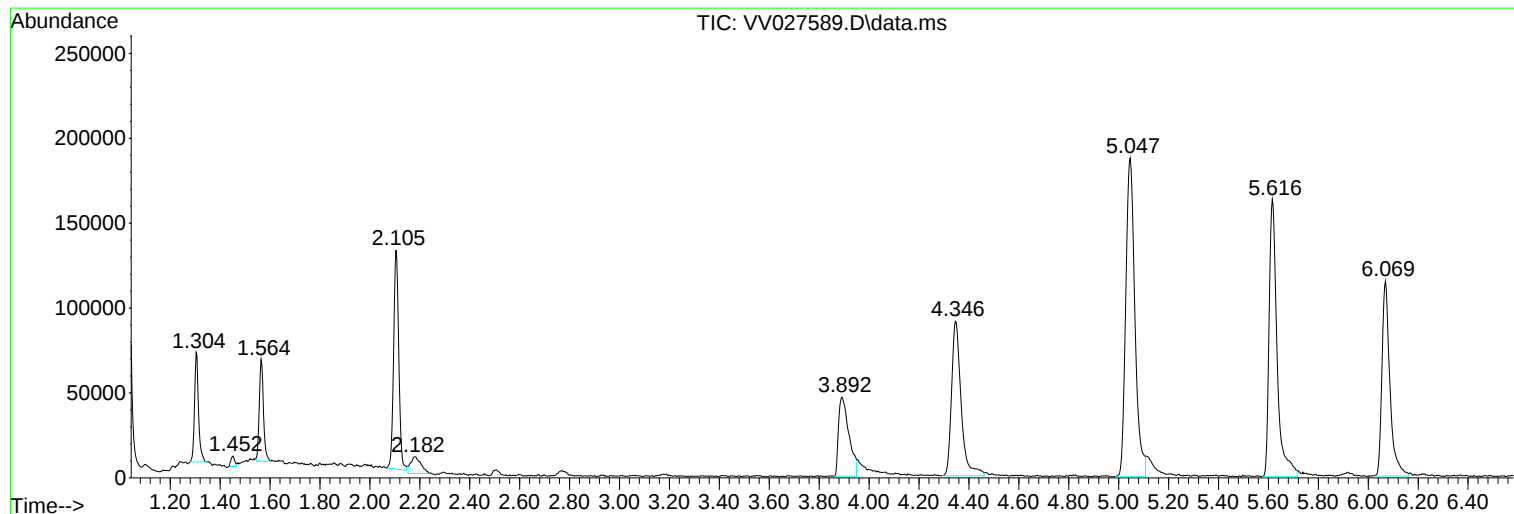

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027589.D
Acq On : 30 Aug 2022 16:27
Operator : SY/MD
Sample : N4404-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVC4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.532	0.61 ug/L	42877	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78

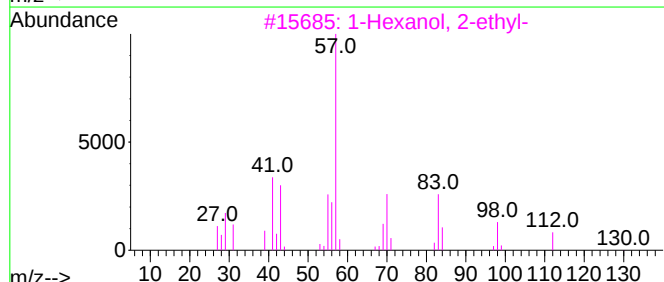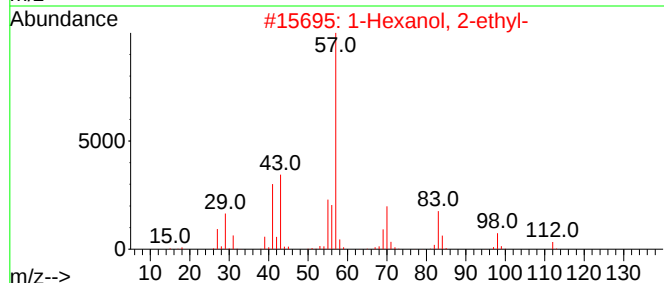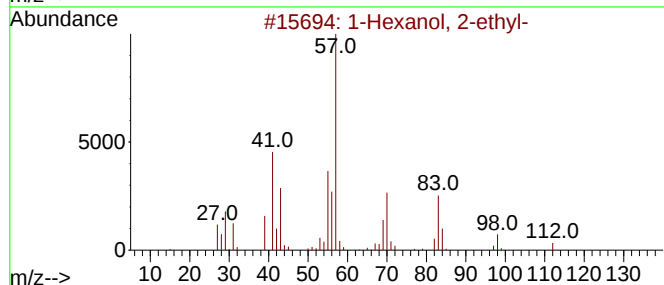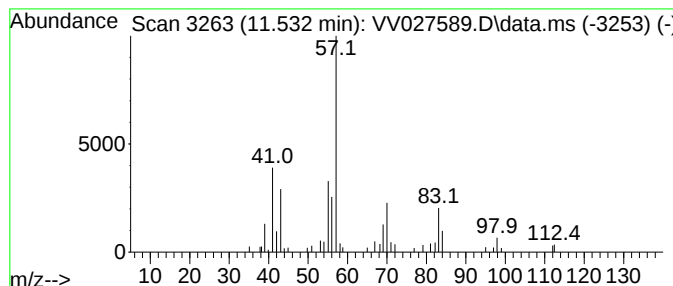

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027589.D
Acq On : 30 Aug 2022 16:27
Operator : SY/MD
Sample : N4404-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.532	0.6	ug/L	42877	3	11.249	353306	5.0