

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027592.D
 Acq On : 30 Aug 2022 17:41
 Operator : SY/MD
 Sample : N4404-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	101	rVB	70929	81588	16.98%	2.031%
2	1.449	123	127	136	rVB2	8341	8337	1.73%	0.208%
3	1.564	156	163	175	rVB	61514	71362	14.85%	1.777%
4	2.105	321	331	345	rVB	130209	186304	38.76%	4.639%
5	2.506	448	456	469	rVB6	3484	5764	1.20%	0.144%
6	2.770	522	538	550	rBV	17444	38998	8.11%	0.971%
7	3.892	874	887	913	rBV2	47089	152145	31.66%	3.788%
8	4.349	1013	1029	1052	rBV	95192	263696	54.86%	6.566%
9	5.047	1231	1246	1264	rBV2	189807	480633	100.00%	11.967%
10	5.616	1409	1423	1456	rBV	155879	349682	72.75%	8.707%
11	6.069	1551	1564	1592	rBV2	119085	263992	54.93%	6.573%
12	6.989	1839	1850	1868	rBV2	38869	78867	16.41%	1.964%
13	7.317	1939	1952	1978	rBV	185976	353421	73.53%	8.800%
14	7.628	2039	2049	2067	rBV2	21676	45364	9.44%	1.129%
15	7.976	2148	2157	2174	rVB3	19015	36491	7.59%	0.909%
16	8.091	2183	2193	2222	rBV	181761	399902	83.20%	9.957%
17	8.853	2418	2430	2460	rBV	251463	434005	90.30%	10.806%
18	10.214	2842	2853	2875	rBV	78774	129073	26.85%	3.214%
19	11.249	3162	3175	3192	rBV	213082	338594	70.45%	8.430%
20	11.535	3255	3264	3280	rBV2	10339	20813	4.33%	0.518%
21	11.622	3280	3291	3309	rVV	172854	277299	57.69%	6.904%




Sum of corrected areas: 4016330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027592.D
Acq On : 30 Aug 2022 17:41
Operator : SY/MD
Sample : N4404-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

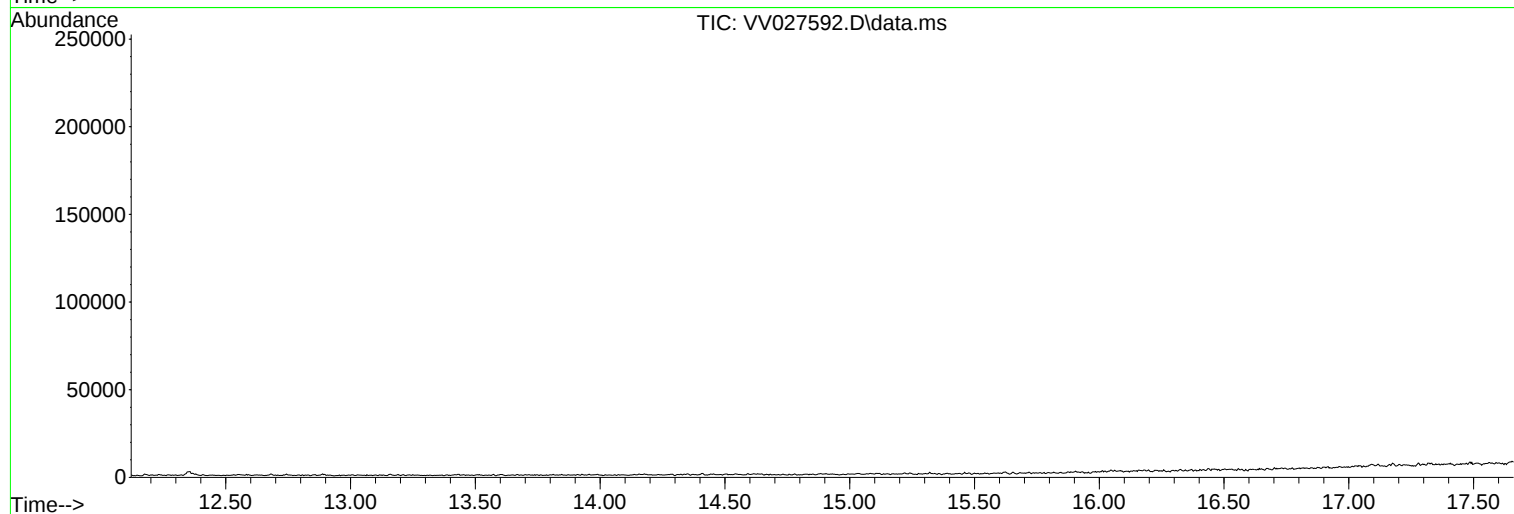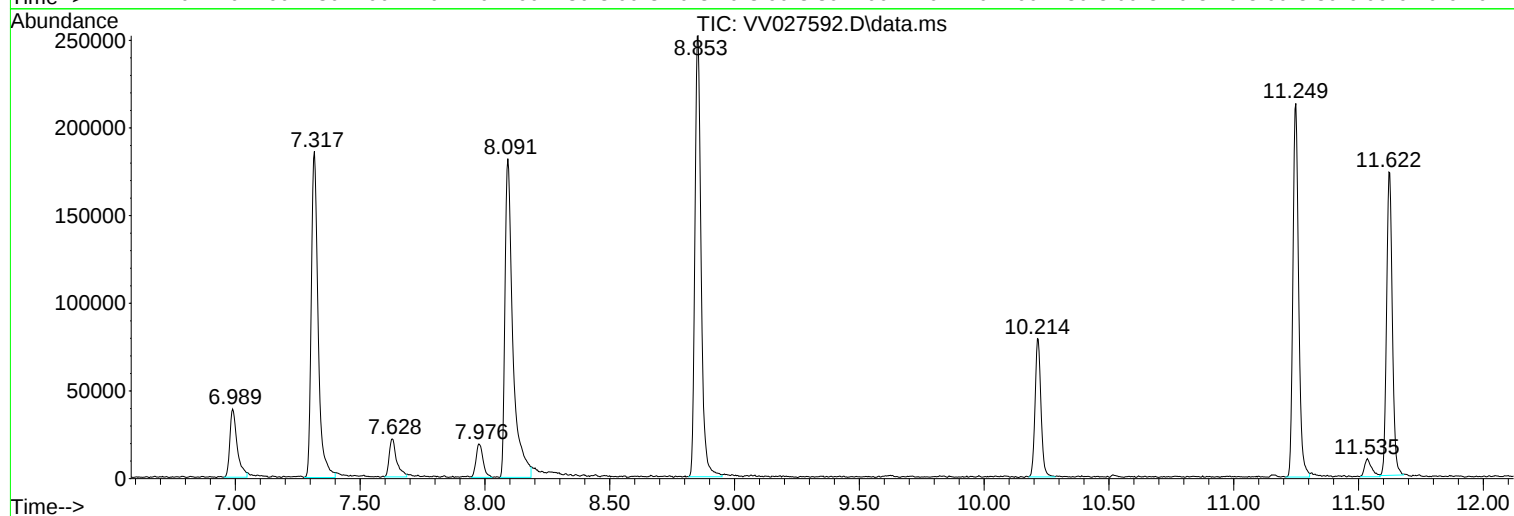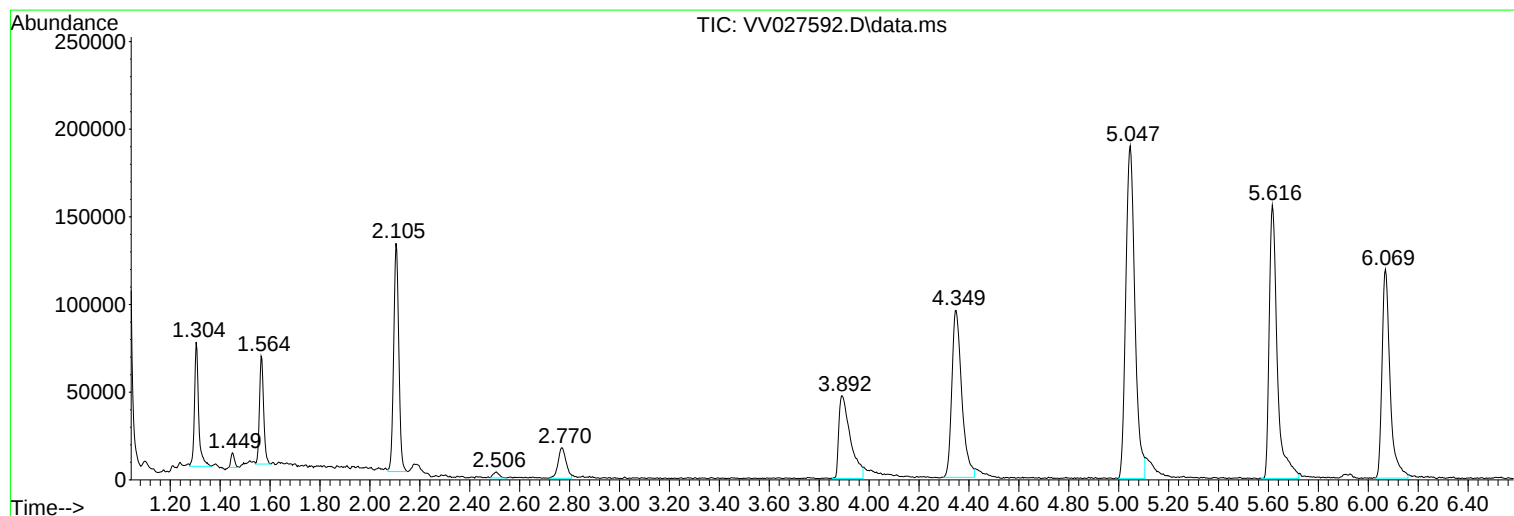

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027592.D
Acq On : 30 Aug 2022 17:41
Operator : SY/MD
Sample : N4404-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027592.D
Acq On : 30 Aug 2022 17:41
Operator : SY/MD
Sample : N4404-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc