
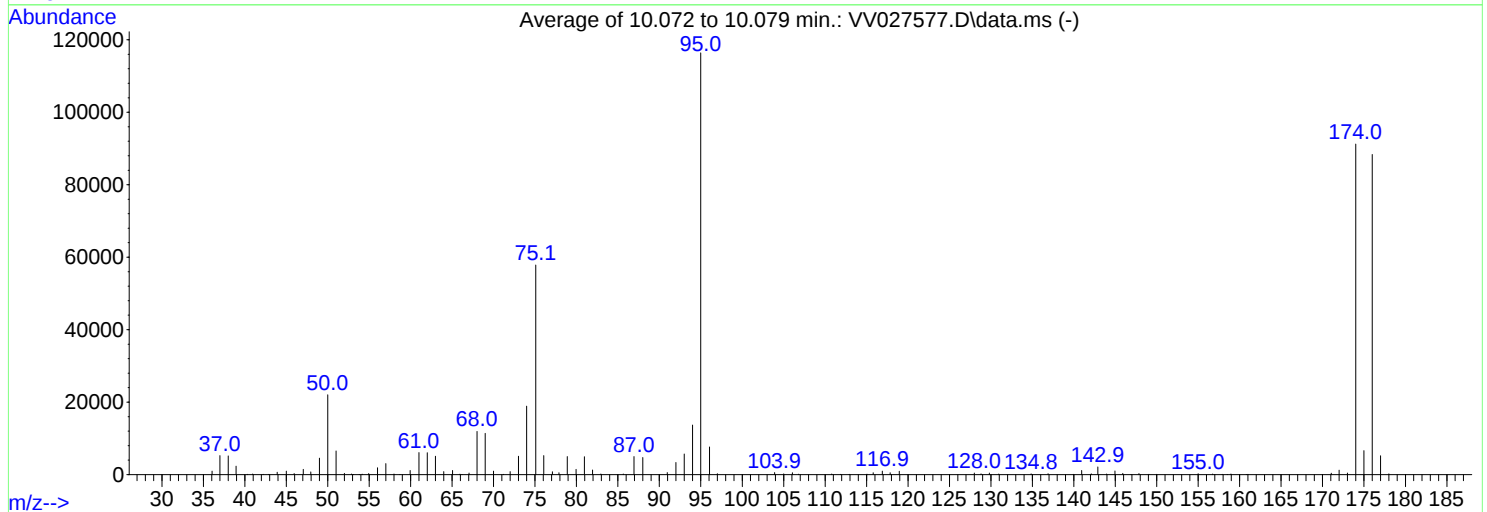


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027577.D
 Acq On : 30 Aug 2022 11:18
 Operator : SY/MD
 Sample : BFB363
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB363

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Sep 01 02:33:10 2022

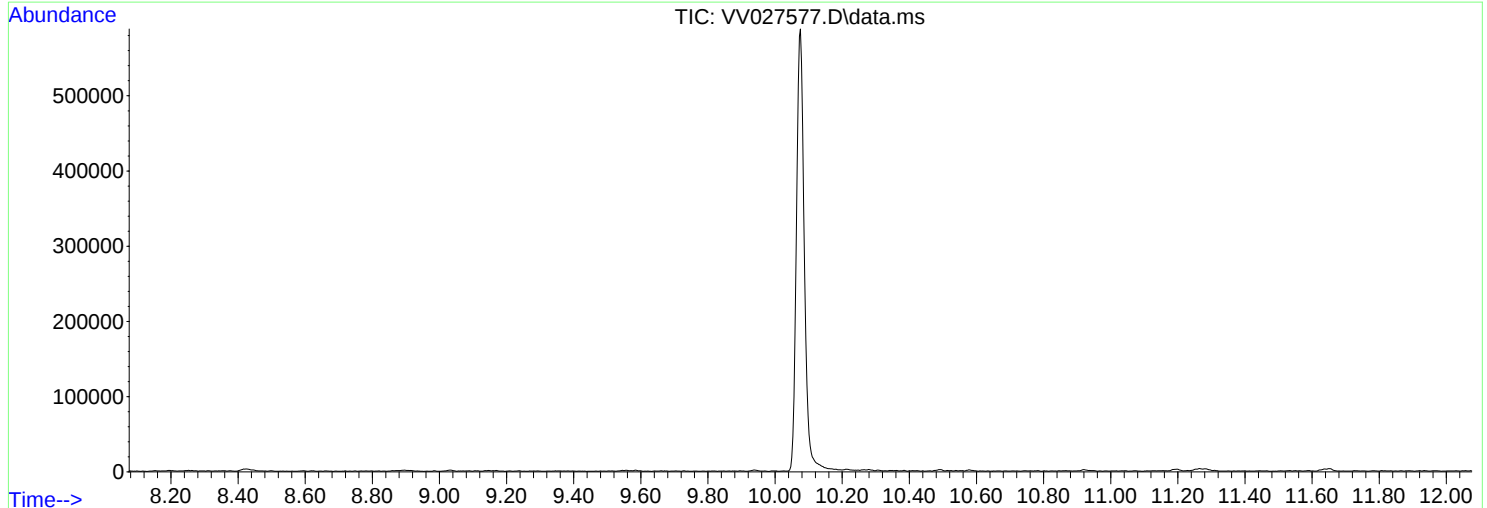

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	22032	PASS
75	95	30	80	49.7	57832	PASS
95	95	100	100	100.0	116395	PASS
96	95	5	9	6.6	7640	PASS
173	174	0.00	2	0.5	430	PASS
174	95	50	120	78.4	91211	PASS
175	174	5	9	7.2	6610	PASS
176	174	95	105	96.9	88352	PASS
177	176	5	10	5.9	5232	PASS

m/z	Abundance
36.10	127.0
38.80	103.0
40.00	279.0
44.00	531.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
36.00	1096.0
37.00	5680.0
38.00	5289.0
39.00	2599.0
40.30	258.0
41.00	175.0
43.90	1251.0
45.00	990.0
45.90	348.0
47.00	1471.0
47.90	727.0
49.00	5004.0
50.00	22336.0
51.00	6708.0
52.00	381.0
52.80	200.0
53.80	119.0
54.10	119.0
55.00	264.0
56.00	1973.0
57.00	3110.0
58.00	179.0
58.70	111.0
60.00	1171.0
61.00	6300.0
62.00	6217.0
63.00	5393.0
63.90	942.0
65.00	1204.0
66.00	177.0
67.10	505.0
68.00	12072.0
69.00	11736.0
70.00	958.0
72.00	822.0
73.00	5340.0
74.00	19160.0
75.10	59080.0
76.00	5339.0
77.10	884.0
78.00	556.0
78.90	5146.0
79.90	1486.0
80.90	5270.0
82.00	1344.0
82.90	167.0
85.60	150.0
87.00	5086.0
88.00	4659.0
91.00	637.0
92.00	3397.0
93.00	5869.0
94.00	13790.0
95.00	118336.0
96.10	8000.0
97.00	264.0
103.90	551.0
105.00	232.0
106.10	517.0
106.80	140.0
110.80	168.0
111.80	136.0
112.90	168.0
115.00	116.0
115.80	554.0
116.90	1013.0
117.80	557.0
118.90	905.0
127.90	470.0
128.70	219.0
129.80	471.0
130.90	184.0
134.90	242.0
136.90	268.0
139.90	127.0
141.00	1121.0
142.10	203.0
142.90	2066.0
143.90	196.0
144.90	1063.0
145.90	312.0
147.90	307.0
155.00	262.0
156.80	199.0
157.90	125.0
158.90	153.0
160.80	167.0
171.10	446.0
172.00	1269.0
173.00	1289.0
174.00	90544.0
175.00	6667.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

176.00	88344.0
177.00	5154.0
178.00	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
36.10	1114.0
37.00	5447.0
38.00	5255.0
39.00	2590.0
41.00	179.0
42.20	120.0
42.90	110.0
43.90	1213.0
45.00	1012.0
46.00	308.0
47.10	1511.0
47.90	725.0
49.00	4583.0
50.00	22816.0
51.00	6716.0
52.00	359.0
52.80	178.0
53.10	173.0
54.20	157.0
54.90	317.0
56.00	1977.0
57.00	3164.0
58.00	192.0
60.00	1179.0
61.00	6326.0
62.00	6314.0
63.00	5200.0
64.00	863.0
65.00	1173.0
65.90	186.0
67.00	460.0
68.00	12240.0
69.00	11594.0
70.00	979.0
71.20	119.0
72.00	853.0
73.00	5159.0
74.00	19360.0
75.10	59864.0
76.10	5372.0
77.10	797.0
77.90	563.0
78.90	5161.0
80.00	1512.0
80.90	5030.0
81.90	1296.0
83.00	217.0
85.70	184.0
86.90	5114.0
88.00	4856.0
90.90	606.0
92.00	3438.0
93.00	5951.0
94.00	14191.0
95.00	120216.0
96.10	7886.0
97.00	292.0
103.90	600.0
105.00	236.0
106.00	546.0
106.80	141.0
110.80	179.0
111.90	105.0
112.90	134.0
115.00	150.0
115.80	537.0
116.90	949.0
117.90	524.0
118.90	959.0
128.00	436.0
128.80	216.0
129.80	431.0
130.90	163.0
134.80	236.0
136.90	273.0
140.00	117.0
141.00	1209.0
142.10	242.0
142.90	2194.0
144.00	177.0
145.00	1040.0
145.90	370.0
147.90	316.0
149.00	117.0
150.00	112.0
155.00	280.0
156.70	198.0
157.00	183.0
157.90	127.0
159.00	175.0
161.00	143.0
171.10	434.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

172.00	1265.0
174.00	94824.0
175.00	6798.0
176.00	91328.0
177.00	5339.0
178.00	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
36.10	1027.0
37.00	4697.0
38.00	4926.0
39.00	2181.0
39.90	343.0
40.90	140.0
42.20	108.0
42.90	123.0
43.90	1077.0
45.00	948.0
46.00	291.0
47.00	1391.0
48.00	770.0
49.00	4116.0
50.00	20944.0
51.00	6191.0
52.00	305.0
52.90	165.0
54.10	177.0
54.90	342.0
56.00	1800.0
57.00	2841.0
58.00	176.0
59.90	1126.0
61.00	5631.0
62.00	5684.0
63.00	4619.0
64.10	780.0
65.10	1027.0
66.20	173.0
67.00	340.0
68.00	11461.0
69.00	10789.0
70.00	939.0
71.20	107.0
72.00	821.0
73.00	4766.0
74.00	18240.0
75.10	54552.0
76.10	5022.0
77.10	651.0
77.80	490.0
78.90	4626.0
80.00	1444.0
81.00	4512.0
81.90	1259.0
83.00	212.0
85.70	236.0
86.90	4794.0
88.00	4682.0
90.90	505.0
92.00	3219.0
93.00	5303.0
94.00	13092.0
95.00	110632.0
96.00	7033.0
97.00	266.0
103.90	587.0
105.00	207.0
106.00	486.0
106.80	130.0
110.80	168.0
115.10	158.0
115.80	491.0
116.90	901.0
117.90	471.0
119.00	945.0
128.10	442.0
128.90	237.0
129.80	426.0
131.00	175.0
134.80	219.0
136.90	239.0
140.90	1163.0
142.10	230.0
142.90	2126.0
144.00	156.0
145.00	911.0
145.90	341.0
146.90	123.0
147.80	268.0
149.10	124.0
150.00	133.0
155.00	269.0
156.70	181.0
158.50	127.0
159.00	170.0
161.00	127.0
171.00	386.0
172.00	1202.0
174.00	88264.0
175.00	6365.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

176.00	85384.0
177.00	5203.0
178.00	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363