

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007309.D
 Acq On : 31 Aug 2018 18:42
 Operator : SY/MD
 Sample : J4695-01DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE41DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.948	9	18	20	rBV2	506	607	0.03%	0.004%
2	1.029	29	43	68	rBV	1489707	1866276	91.53%	10.980%
3	1.321	127	134	151	rVB	226434	270930	13.29%	1.594%
4	1.575	208	213	228	rVB	184889	223970	10.98%	1.318%
5	2.131	377	386	398	rVB	440925	614005	30.11%	3.612%
6	3.434	789	791	795	rBV	736	491	0.02%	0.003%
7	3.556	826	829	834	rBV2	607	373	0.02%	0.002%
8	3.745	883	888	890	rBV3	561	527	0.03%	0.003%
9	3.794	902	903	910	rVB2	545	451	0.02%	0.003%
10	3.858	921	923	927	rVB2	464	312	0.02%	0.002%
11	3.964	939	956	1006	rBV	150695	483964	23.74%	2.847%
12	4.257	1043	1047	1051	rBV3	480	386	0.02%	0.002%
13	4.279	1052	1054	1059	rVB4	660	503	0.02%	0.003%
14	4.305	1059	1062	1063	rBV	489	320	0.02%	0.002%
15	4.408	1077	1094	1122	rBV	335920	798017	39.14%	4.695%
16	4.733	1188	1195	1196	rBV3	593	539	0.03%	0.003%
17	4.758	1196	1203	1206	rVV5	651	859	0.04%	0.005%
18	4.871	1235	1238	1242	rBV3	451	349	0.02%	0.002%
19	4.922	1252	1254	1259	rVB2	527	435	0.02%	0.003%
20	5.102	1289	1310	1348	rBV2	847837	2038900	100.00%	11.995%
21	5.289	1366	1368	1370	rVB3	647	280	0.01%	0.002%
22	5.334	1377	1382	1384	rBV5	559	409	0.02%	0.002%
23	5.379	1391	1396	1398	rVB3	669	486	0.02%	0.003%
24	5.446	1412	1417	1423	rVV6	579	687	0.03%	0.004%
25	5.488	1428	1430	1433	rVB3	428	272	0.01%	0.002%
26	5.507	1433	1436	1439	rBV3	434	299	0.01%	0.002%
27	5.556	1450	1451	1455	rVB3	449	281	0.01%	0.002%
28	5.581	1455	1459	1461	rBV2	586	416	0.02%	0.002%
29	5.671	1470	1487	1520	rBV	687987	1384542	67.91%	8.146%
30	5.813	1527	1531	1535	rVB3	1060	790	0.04%	0.005%
31	5.839	1535	1539	1541	rBV3	738	576	0.03%	0.003%
32	5.964	1564	1578	1592	rVB6	24723	52023	2.55%	0.306%
33	6.019	1592	1595	1597	rBV4	432	279	0.01%	0.002%
34	6.125	1612	1628	1656	rBV	469003	951382	46.66%	5.597%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007309.D
 Acq On : 31 Aug 2018 18:42
 Operator : SY/MD
 Sample : J4695-01DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE41DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.334	1690	1693	1695	rBV3	456	316	0.02%	0.002%
36	6.363	1699	1702	1704	rBV2	464	272	0.01%	0.002%
37	6.376	1704	1706	1711	rVB3	535	424	0.02%	0.002%
38	6.655	1789	1793	1796	rVV3	1290	1014	0.05%	0.006%
39	6.671	1796	1798	1802	rVB4	949	598	0.03%	0.004%
40	6.732	1806	1817	1829	rBV4	3560	8605	0.42%	0.051%
41	6.806	1838	1840	1845	rVB2	484	350	0.02%	0.002%
42	6.964	1887	1889	1895	rBV2	388	384	0.02%	0.002%
43	7.035	1896	1911	1932	rBV	224063	408744	20.05%	2.405%
44	7.173	1950	1954	1962	rVB7	806	1046	0.05%	0.006%
45	7.263	1979	1982	1984	rBV3	422	314	0.02%	0.002%
46	7.282	1985	1988	1991	rBV3	549	340	0.02%	0.002%
47	7.302	1992	1994	1999	rVB2	542	408	0.02%	0.002%
48	7.366	1999	2014	2046	rBV	859760	1507520	73.94%	8.869%
49	7.668	2097	2108	2125	rVV	161271	278068	13.64%	1.636%
50	7.790	2143	2146	2148	rBV4	670	539	0.03%	0.003%
51	8.022	2210	2218	2229	rVB3	31888	53779	2.64%	0.316%
52	8.096	2239	2241	2243	rBV	468	303	0.01%	0.002%
53	8.144	2244	2256	2289	rBV	494052	917226	44.99%	5.396%
54	8.511	2367	2370	2375	rVB4	489	434	0.02%	0.003%
55	8.581	2388	2392	2396	rBV3	779	686	0.03%	0.004%
56	8.700	2425	2429	2431	rVB2	465	348	0.02%	0.002%
57	8.784	2449	2455	2459	rVB4	700	797	0.04%	0.005%
58	8.822	2459	2467	2470	rBV3	972	1340	0.07%	0.008%
59	8.900	2478	2491	2513	rBV	1012243	1638642	80.37%	9.641%
60	9.138	2562	2565	2570	rVB3	473	399	0.02%	0.002%
61	9.186	2575	2580	2581	rBV3	1036	853	0.04%	0.005%
62	9.240	2594	2597	2601	rVB2	531	379	0.02%	0.002%
63	9.266	2601	2605	2607	rBV4	449	306	0.02%	0.002%
64	9.369	2632	2637	2641	rBV4	513	443	0.02%	0.003%
65	9.494	2673	2676	2677	rBV	607	331	0.02%	0.002%
66	9.745	2751	2754	2755	rBV3	456	267	0.01%	0.002%
67	9.803	2767	2772	2777	rVB4	510	578	0.03%	0.003%
68	9.864	2788	2791	2795	rBV2	497	383	0.02%	0.002%
69	9.977	2823	2826	2830	rVB4	825	578	0.03%	0.003%
70	10.019	2837	2839	2843	rVB2	546	349	0.02%	0.002%
71	10.067	2849	2854	2857	rBV2	655	606	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007309.D
 Acq On : 31 Aug 2018 18:42
 Operator : SY/MD
 Sample : J4695-01DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE41DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	10.099	2862	2864	2870	rVB3	484	393	0.02%	0.002%
73	10.134	2870	2875	2876	rBV2	360	313	0.02%	0.002%
74	10.266	2903	2916	2932	rBV	624018	993186	48.71%	5.843%
75	10.427	2960	2966	2967	rBV4	1465	1411	0.07%	0.008%
76	10.597	3015	3019	3021	rBV2	315	317	0.02%	0.002%
77	10.655	3035	3037	3043	rBV2	435	276	0.01%	0.002%
78	10.684	3043	3046	3051	rVB2	487	379	0.02%	0.002%
79	10.719	3051	3057	3059	rBV3	532	531	0.03%	0.003%
80	10.761	3068	3070	3075	rVB3	568	357	0.02%	0.002%
81	10.845	3090	3096	3098	rBV2	440	420	0.02%	0.002%
82	10.906	3111	3115	3119	rBV3	436	498	0.02%	0.003%
83	11.009	3144	3147	3152	rVB3	912	687	0.03%	0.004%
84	11.057	3158	3162	3165	rBV	582	476	0.02%	0.003%
85	11.157	3190	3193	3195	rBV	423	284	0.01%	0.002%
86	11.231	3207	3216	3221	rBV7	1575	2783	0.14%	0.016%
87	11.298	3225	3237	3268	rBV	768522	1232221	60.44%	7.249%
88	11.427	3274	3277	3280	rBV3	485	282	0.01%	0.002%
89	11.536	3308	3311	3314	rVV3	855	687	0.03%	0.004%
90	11.578	3316	3324	3342	rVV5	9711	21764	1.07%	0.128%
91	11.678	3342	3355	3379	rVB	754501	1211156	59.40%	7.126%
92	11.893	3419	3422	3425	rBV2	393	305	0.01%	0.002%
93	12.295	3545	3547	3554	rVB4	541	501	0.02%	0.003%
94	12.465	3597	3600	3605	rBV4	790	713	0.03%	0.004%
95	13.086	3790	3793	3797	rBV2	758	630	0.03%	0.004%
96	13.215	3830	3833	3837	rBV4	871	719	0.04%	0.004%
97	13.523	3927	3929	3932	rBV3	741	411	0.02%	0.002%
98	13.797	4011	4014	4017	rBV3	1228	1009	0.05%	0.006%
99	13.996	4073	4076	4079	rBV3	879	736	0.04%	0.004%
100	14.481	4224	4227	4233	rBV5	1241	1032	0.05%	0.006%


Sum of corrected areas: 16997382

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007309.D
Acq On : 31 Aug 2018 18:42
Operator : SY/MD
Sample : J4695-01DL 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE41DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

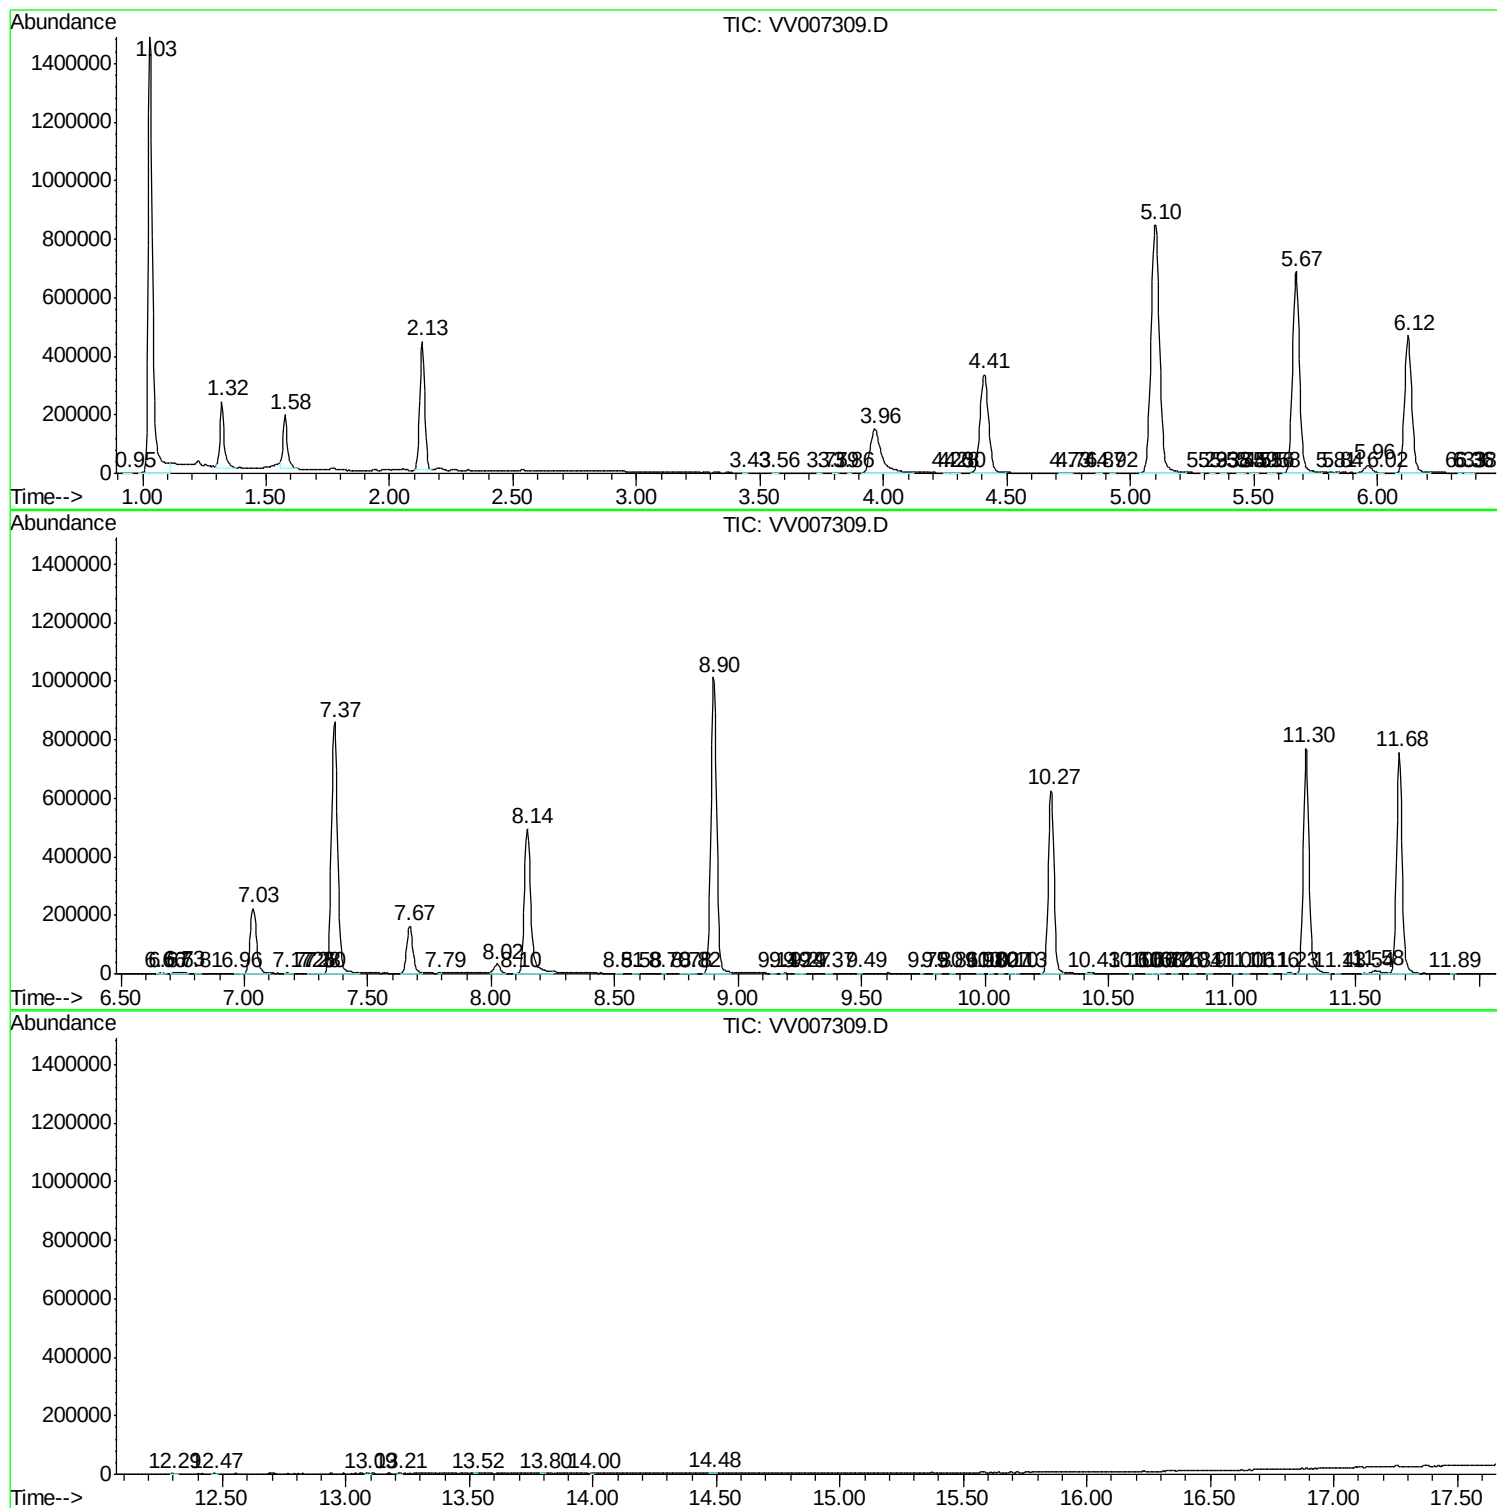

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007309.D
Acq On : 31 Aug 2018 18:42
Operator : SY/MD
Sample : J4695-01DL 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE41DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV083118\
Data File : VV007309.D
Acq On : 31 Aug 2018 18:42
Operator : SY/MD
Sample : J4695-01DL 50X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEE41DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc