

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007310.D
 Acq On : 31 Aug 2018 19:07
 Operator : SY/MD
 Sample : J4695-02DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.951	17	19	25	rVB3	629	594	0.03%	0.004%
2	0.984	25	29	30	rBV	328	222	0.01%	0.001%
3	1.029	30	43	64	rBV	1482841	1809817	88.98%	10.923%
4	1.321	128	134	153	rVB	222054	264129	12.99%	1.594%
5	1.575	208	213	238	rVB	188062	241536	11.88%	1.458%
6	2.131	376	386	398	rBV	436944	608991	29.94%	3.676%
7	3.475	801	804	805	rBV	622	339	0.02%	0.002%
8	3.659	859	861	865	rVB2	578	345	0.02%	0.002%
9	3.781	896	899	900	rBV	440	273	0.01%	0.002%
10	3.832	910	915	920	rBV3	517	455	0.02%	0.003%
11	3.871	924	927	929	rBV3	510	326	0.02%	0.002%
12	3.903	934	937	939	rBV2	359	257	0.01%	0.002%
13	3.964	939	956	994	rBV	163166	522847	25.71%	3.156%
14	4.250	1043	1045	1047	rBV2	432	250	0.01%	0.002%
15	4.408	1076	1094	1125	rBV	336642	806846	39.67%	4.870%
16	4.588	1147	1150	1152	rBV3	441	322	0.02%	0.002%
17	4.620	1158	1160	1165	rBV4	544	427	0.02%	0.003%
18	4.701	1183	1185	1189	rBV2	404	312	0.02%	0.002%
19	4.720	1189	1191	1197	rBV3	339	338	0.02%	0.002%
20	4.848	1228	1231	1234	rBV3	416	289	0.01%	0.002%
21	4.881	1238	1241	1243	rBV	309	224	0.01%	0.001%
22	4.977	1266	1271	1273	rBV2	257	250	0.01%	0.002%
23	5.099	1289	1309	1343	rBV2	842893	2033947	100.00%	12.276%
24	5.456	1411	1420	1424	rBV4	642	929	0.05%	0.006%
25	5.524	1439	1441	1444	rVV	403	228	0.01%	0.001%
26	5.598	1459	1464	1466	rBV3	458	296	0.01%	0.002%
27	5.614	1466	1469	1470	rBV2	371	233	0.01%	0.001%
28	5.672	1471	1487	1520	rBV	652147	1304895	64.16%	7.876%
29	5.958	1564	1576	1592	rVB6	12769	29206	1.44%	0.176%
30	6.125	1612	1628	1658	rBV	477402	954833	46.94%	5.763%
31	6.450	1727	1729	1732	rBV2	512	314	0.02%	0.002%
32	6.520	1748	1751	1752	rBV2	572	325	0.02%	0.002%
33	6.598	1771	1775	1779	rVB2	403	286	0.01%	0.002%
34	6.620	1779	1782	1784	rBV2	507	312	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007310.D
 Acq On : 31 Aug 2018 19:07
 Operator : SY/MD
 Sample : J4695-02DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.655	1787	1793	1794	rBV3	892	798	0.04%	0.005%
36	6.736	1807	1818	1830	rBV4	4443	9603	0.47%	0.058%
37	6.948	1881	1884	1892	rVB3	593	621	0.03%	0.004%
38	6.987	1892	1896	1897	rBV3	501	325	0.02%	0.002%
39	7.035	1897	1911	1940	rVV	223396	408841	20.10%	2.468%
40	7.270	1982	1984	1988	rBV2	609	396	0.02%	0.002%
41	7.366	2000	2014	2033	rBV	825699	1444917	71.04%	8.721%
42	7.668	2094	2108	2130	rBV	161831	281389	13.83%	1.698%
43	8.022	2210	2218	2228	rVB3	14966	25586	1.26%	0.154%
44	8.077	2232	2235	2239	rVB3	740	447	0.02%	0.003%
45	8.144	2243	2256	2277	rBV	513548	939861	46.21%	5.673%
46	8.546	2377	2381	2385	rBV4	796	772	0.04%	0.005%
47	8.623	2403	2405	2406	rBV	455	240	0.01%	0.001%
48	8.704	2427	2430	2435	rBV3	529	408	0.02%	0.002%
49	8.729	2435	2438	2441	rVV3	358	281	0.01%	0.002%
50	8.784	2452	2455	2458	rBV3	384	342	0.02%	0.002%
51	8.829	2467	2469	2471	rBV3	379	230	0.01%	0.001%
52	8.900	2475	2491	2514	rBV	938207	1524306	74.94%	9.200%
53	9.118	2555	2559	2564	rVB6	1173	1274	0.06%	0.008%
54	9.157	2569	2571	2575	rBV4	569	536	0.03%	0.003%
55	9.183	2577	2579	2580	rBV	540	247	0.01%	0.001%
56	9.279	2606	2609	2610	rBV2	616	309	0.02%	0.002%
57	9.302	2613	2616	2620	rVB3	549	380	0.02%	0.002%
58	9.343	2627	2629	2633	rVB2	485	281	0.01%	0.002%
59	9.385	2633	2642	2647	rBV4	689	1283	0.06%	0.008%
60	9.427	2653	2655	2660	rVB2	367	227	0.01%	0.001%
61	9.472	2666	2669	2671	rBV	529	416	0.02%	0.003%
62	9.530	2685	2687	2690	rBV2	319	229	0.01%	0.001%
63	9.591	2703	2706	2707	rVV2	738	370	0.02%	0.002%
64	9.607	2709	2711	2717	rVB5	833	775	0.04%	0.005%
65	9.662	2725	2728	2731	rBV3	367	249	0.01%	0.002%
66	9.697	2736	2739	2742	rVV3	578	452	0.02%	0.003%
67	9.961	2817	2821	2825	rBV2	544	526	0.03%	0.003%
68	9.980	2825	2827	2831	rVV3	452	268	0.01%	0.002%
69	10.070	2853	2855	2858	rVB2	492	247	0.01%	0.001%
70	10.096	2859	2863	2864	rBV	327	222	0.01%	0.001%
71	10.138	2872	2876	2882	rVB5	576	640	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007310.D
 Acq On : 31 Aug 2018 19:07
 Operator : SY/MD
 Sample : J4695-02DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	10.179	2886	2889	2892	rBV	540	393	0.02%	0.002%
73	10.266	2904	2916	2938	rBV	633244	1005134	49.42%	6.066%
74	10.430	2960	2967	2976	rVB3	2152	3012	0.15%	0.018%
75	10.633	3025	3030	3032	rBV3	468	352	0.02%	0.002%
76	10.646	3032	3034	3037	rVB	473	257	0.01%	0.002%
77	10.694	3047	3049	3053	rVB	341	249	0.01%	0.002%
78	10.726	3057	3059	3062	rVB2	515	300	0.01%	0.002%
79	10.829	3086	3091	3094	rBV2	430	426	0.02%	0.003%
80	10.848	3094	3097	3100	rVB3	544	312	0.02%	0.002%
81	10.903	3110	3114	3119	rVB4	936	875	0.04%	0.005%
82	11.067	3162	3165	3168	rBV3	412	363	0.02%	0.002%
83	11.134	3184	3186	3190	rBV3	302	238	0.01%	0.001%
84	11.189	3199	3203	3204	rBV2	461	263	0.01%	0.002%
85	11.202	3205	3207	3209	rVV2	546	228	0.01%	0.001%
86	11.231	3211	3216	3224	rVB5	1322	1663	0.08%	0.010%
87	11.298	3224	3237	3262	rBV	702606	1140373	56.07%	6.883%
88	11.527	3302	3308	3310	rBV3	498	587	0.03%	0.004%
89	11.575	3318	3323	3325	rBV3	2182	2049	0.10%	0.012%
90	11.678	3341	3355	3378	rBV	727341	1172903	57.67%	7.079%
91	11.867	3412	3414	3419	rBV3	359	285	0.01%	0.002%
92	11.993	3449	3453	3456	rBV4	655	537	0.03%	0.003%
93	12.144	3498	3500	3503	rVB	602	235	0.01%	0.001%
94	12.292	3544	3546	3551	rVB4	871	514	0.03%	0.003%
95	12.343	3560	3562	3565	rBV3	571	406	0.02%	0.002%
96	12.510	3610	3614	3618	rBV4	732	728	0.04%	0.004%
97	12.703	3668	3674	3684	rVB7	897	1481	0.07%	0.009%
98	12.835	3713	3715	3717	rBV2	614	280	0.01%	0.002%
99	12.977	3756	3759	3761	rBV3	489	270	0.01%	0.002%
100	13.449	3903	3906	3909	rBV3	602	445	0.02%	0.003%


Sum of corrected areas: 16568645

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007310.D
Acq On : 31 Aug 2018 19:07
Operator : SY/MD
Sample : J4695-02DL 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE43DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

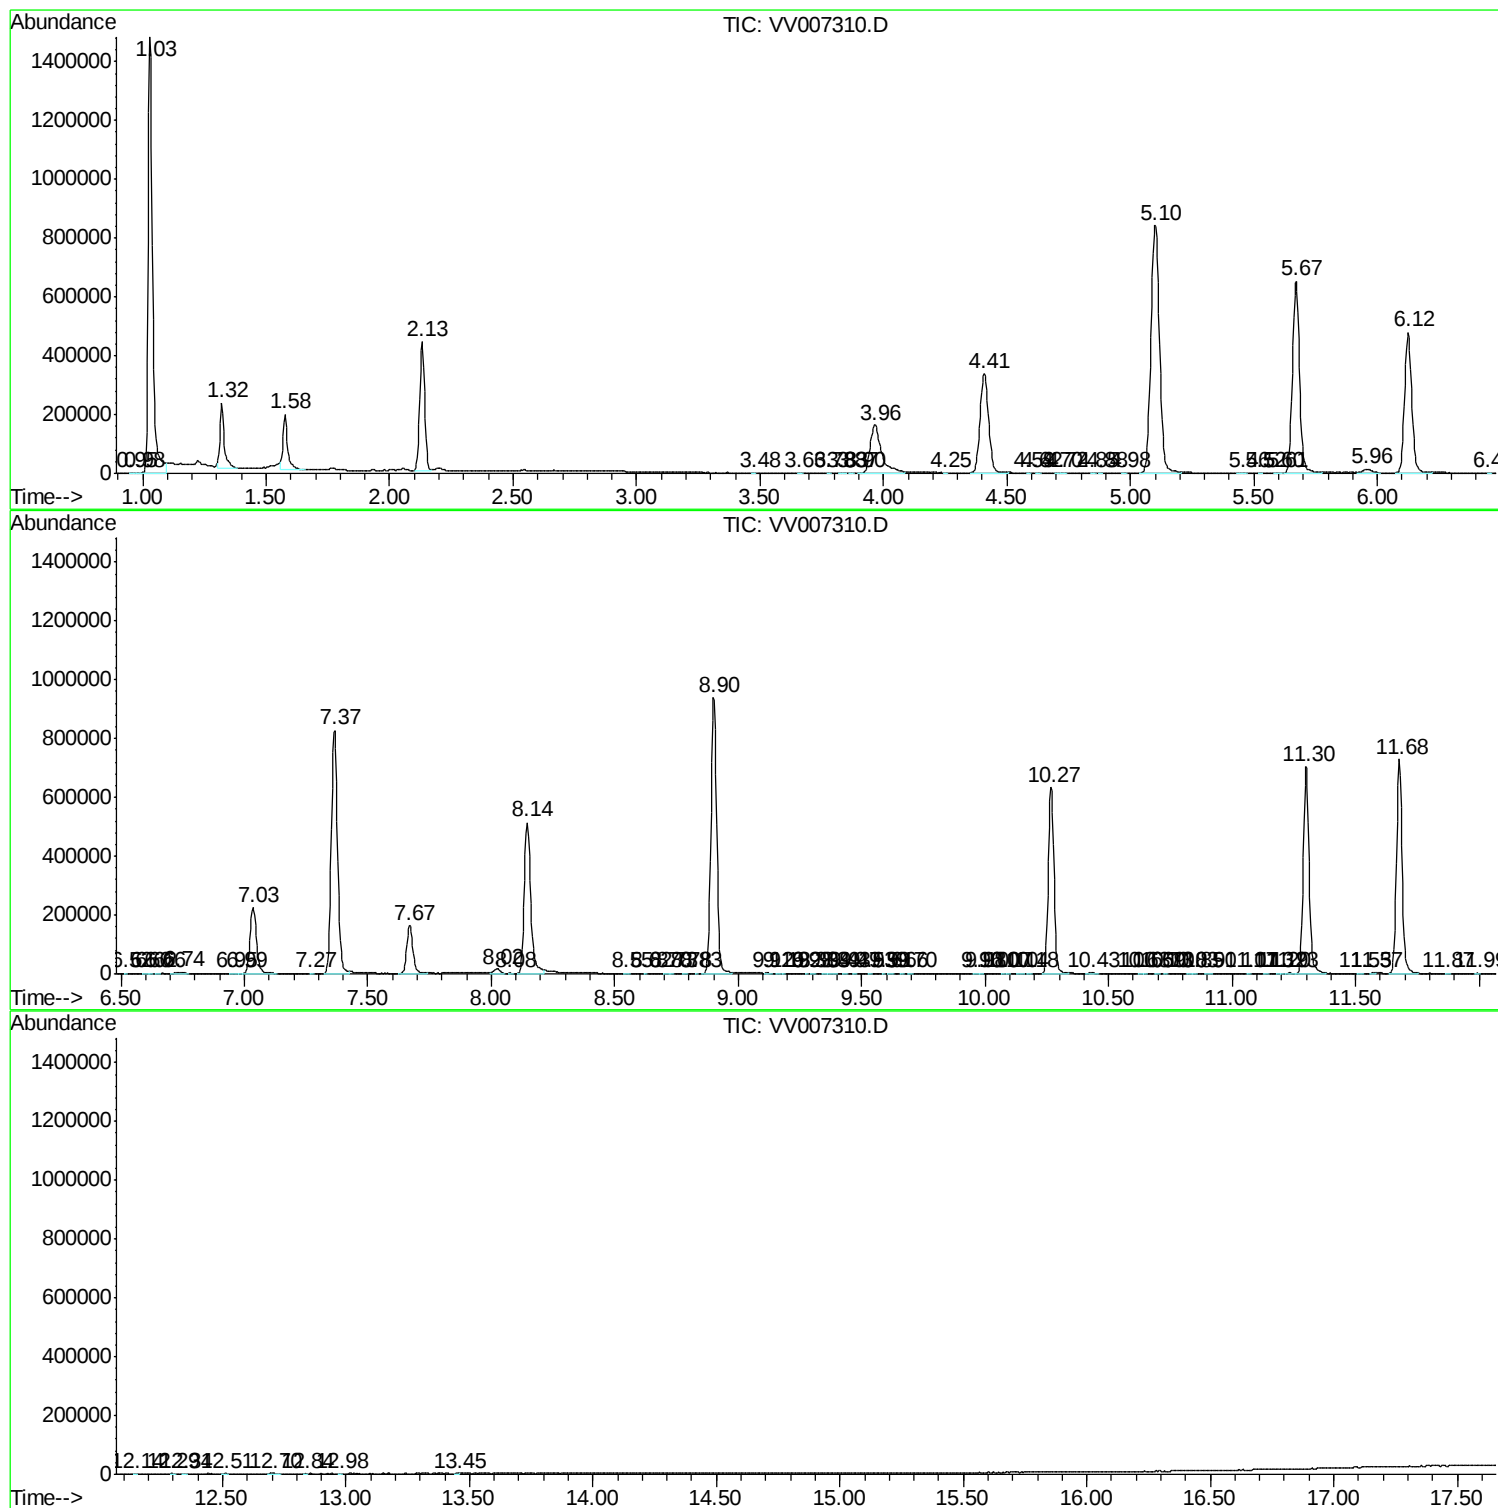

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007310.D
Acq On : 31 Aug 2018 19:07
Operator : SY/MD
Sample : J4695-02DL 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE43DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV083118\
Data File : VV007310.D
Acq On : 31 Aug 2018 19:07
Operator : SY/MD
Sample : J4695-02DL 50X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEE43DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc