

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007311.D
 Acq On : 31 Aug 2018 19:31
 Operator : SY/MD
 Sample : J4695-03DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.939	12	15	18	rBV2	540	346	0.002%	0.0002%
2	1.029	29	43	65	rBV	1578729	1922260	94.48%	11.456%
3	1.321	127	134	150	rVB	222009	258000	12.68%	1.538%
4	1.575	207	213	234	rVB	186011	242215	11.90%	1.443%
5	2.132	376	386	397	rBV	438673	615812	30.27%	3.670%
6	3.443	792	794	799	rVB	606	407	0.002%	0.0002%
7	3.482	803	806	807	rBV	529	306	0.002%	0.0002%
8	3.562	824	831	836	rBV3	688	939	0.005%	0.0006%
9	3.685	865	869	871	rBV2	460	310	0.002%	0.0002%
10	3.826	905	913	917	rBV	466	585	0.003%	0.0003%
11	3.865	922	925	930	rVB2	384	280	0.001%	0.0002%
12	3.964	938	956	1007	rBV	147645	502742	24.71%	2.996%
13	4.283	1050	1055	1059	rBV4	517	514	0.003%	0.0003%
14	4.312	1062	1064	1068	rVB4	584	334	0.002%	0.0002%
15	4.334	1068	1071	1075	rVB4	431	318	0.002%	0.0002%
16	4.408	1075	1094	1118	rBV	336744	811281	39.87%	4.835%
17	4.594	1148	1152	1153	rBV3	727	509	0.003%	0.0003%
18	4.620	1158	1160	1166	rVB2	590	440	0.002%	0.0003%
19	4.730	1190	1194	1196	rBV4	423	318	0.002%	0.0002%
20	4.897	1241	1246	1250	rVV	404	441	0.002%	0.0003%
21	5.099	1290	1309	1347	rBV2	851126	2034598	100.00%	12.125%
22	5.279	1363	1365	1368	rVB3	606	314	0.002%	0.0002%
23	5.453	1416	1419	1424	rVB4	807	566	0.003%	0.0003%
24	5.562	1450	1453	1456	rBV2	439	377	0.002%	0.0002%
25	5.672	1471	1487	1515	rBV	664711	1337974	65.76%	7.974%
26	5.948	1569	1573	1574	rBV3	5225	3516	0.017%	0.0021%
27	6.125	1612	1628	1653	rBV	468082	947836	46.59%	5.649%
28	6.401	1712	1714	1717	rVB	575	278	0.001%	0.0002%
29	6.492	1738	1742	1745	rBV3	418	309	0.002%	0.0002%
30	6.549	1757	1760	1765	rVB4	407	389	0.002%	0.0002%
31	6.643	1786	1789	1790	rBV3	894	547	0.003%	0.0003%
32	6.681	1799	1801	1806	rVB2	414	316	0.002%	0.0002%
33	6.739	1806	1819	1830	rBV	4673	10465	0.51%	0.0062%
34	6.932	1873	1879	1880	rBV3	533	513	0.003%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007311.D
 Acq On : 31 Aug 2018 19:31
 Operator : SY/MD
 Sample : J4695-03DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.967	1887	1890	1893	rBV2	402	326	0.02%	0.002%
36	7.035	1896	1911	1930	rBV	224840	403939	19.85%	2.407%
37	7.308	1994	1996	1999	rVB2	881	455	0.02%	0.003%
38	7.366	1999	2014	2035	rBV	851950	1484888	72.98%	8.849%
39	7.533	2064	2066	2072	rVB4	678	583	0.03%	0.003%
40	7.623	2092	2094	2096	rBV2	705	415	0.02%	0.002%
41	7.668	2096	2108	2128	rVV	162108	281575	13.84%	1.678%
42	7.829	2156	2158	2161	rBV3	780	421	0.02%	0.003%
43	8.022	2209	2218	2229	rVB3	13684	24550	1.21%	0.146%
44	8.096	2237	2241	2242	rBV	1024	587	0.03%	0.003%
45	8.147	2244	2257	2290	rVV	508326	936535	46.03%	5.581%
46	8.556	2381	2384	2387	rVB4	595	319	0.02%	0.002%
47	8.591	2391	2395	2400	rBV4	478	576	0.03%	0.003%
48	8.614	2400	2402	2405	rVV2	446	293	0.01%	0.002%
49	8.639	2406	2410	2413	rVV4	482	430	0.02%	0.003%
50	8.659	2413	2416	2417	rVV	534	283	0.01%	0.002%
51	8.671	2417	2420	2421	rVV2	632	374	0.02%	0.002%
52	8.697	2424	2428	2433	rVB2	639	557	0.03%	0.003%
53	8.768	2448	2450	2455	rVB3	743	537	0.03%	0.003%
54	8.816	2460	2465	2467	rBV3	553	593	0.03%	0.004%
55	8.900	2475	2491	2522	rBV	970502	1581626	77.74%	9.426%
56	9.122	2556	2560	2563	rVB5	1266	874	0.04%	0.005%
57	9.234	2592	2595	2598	rBV2	499	352	0.02%	0.002%
58	9.253	2599	2601	2604	rVV2	641	399	0.02%	0.002%
59	9.279	2606	2609	2613	rVV4	497	484	0.02%	0.003%
60	9.321	2620	2622	2627	rVB2	411	280	0.01%	0.002%
61	9.369	2634	2637	2643	rVB3	497	531	0.03%	0.003%
62	9.469	2664	2668	2672	rBV	401	357	0.02%	0.002%
63	9.495	2672	2676	2679	rVB2	529	412	0.02%	0.002%
64	9.546	2688	2692	2694	rBV	485	400	0.02%	0.002%
65	9.597	2700	2708	2709	rBV3	529	649	0.03%	0.004%
66	9.610	2709	2712	2716	rVB2	947	680	0.03%	0.004%
67	9.633	2716	2719	2723	rBV4	588	567	0.03%	0.003%
68	9.668	2727	2730	2735	rVB4	401	330	0.02%	0.002%
69	9.868	2790	2792	2799	rVB3	432	338	0.02%	0.002%
70	9.903	2799	2803	2808	rBV2	472	448	0.02%	0.003%
71	9.964	2817	2822	2824	rVV3	432	433	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007311.D
 Acq On : 31 Aug 2018 19:31
 Operator : SY/MD
 Sample : J4695-03DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	9.980	2825	2827	2832	rVB	544	352	0.02%	0.002%
73	10.125	2866	2872	2876	rBV3	513	478	0.02%	0.003%
74	10.212	2896	2899	2903	rVB	626	358	0.02%	0.002%
75	10.266	2903	2916	2933	rBV	621636	994818	48.90%	5.929%
76	10.430	2962	2967	2979	rVB3	1858	2735	0.13%	0.016%
77	10.475	2979	2981	2986	rVB	521	451	0.02%	0.003%
78	10.565	3005	3009	3013	rVB2	414	333	0.02%	0.002%
79	10.694	3045	3049	3054	rVV3	339	422	0.02%	0.003%
80	10.906	3112	3115	3121	rVB5	882	998	0.05%	0.006%
81	11.028	3147	3153	3159	rVB4	652	921	0.05%	0.005%
82	11.060	3159	3163	3164	rBV2	442	309	0.02%	0.002%
83	11.170	3194	3197	3202	rBV2	374	288	0.01%	0.002%
84	11.224	3211	3214	3215	rBV2	822	466	0.02%	0.003%
85	11.298	3225	3237	3265	rBV	721927	1163716	57.20%	6.935%
86	11.404	3265	3270	3272	rVB5	479	433	0.02%	0.003%
87	11.433	3276	3279	3280	rBV3	504	330	0.02%	0.002%
88	11.575	3320	3323	3325	rBV2	1164	909	0.04%	0.005%
89	11.678	3342	3355	3380	rBV	730005	1182745	58.13%	7.049%
90	11.768	3380	3383	3386	rVB3	710	433	0.02%	0.003%
91	11.787	3386	3389	3392	rVB3	695	446	0.02%	0.003%
92	11.900	3421	3424	3427	rBV2	477	327	0.02%	0.002%
93	11.974	3443	3447	3450	rBV	333	285	0.01%	0.002%
94	12.080	3477	3480	3483	rVB3	820	586	0.03%	0.003%
95	12.331	3555	3558	3562	rBV2	565	508	0.02%	0.003%
96	12.369	3567	3570	3572	rBV2	615	335	0.02%	0.002%
97	12.691	3668	3670	3673	rBV3	752	498	0.02%	0.003%
98	12.777	3694	3697	3700	rBV3	333	277	0.01%	0.002%
99	12.819	3707	3710	3715	rBV3	558	601	0.03%	0.004%
100	13.488	3915	3918	3922	rBV5	1088	931	0.05%	0.006%


Sum of corrected areas: 16780040

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007311.D
Acq On : 31 Aug 2018 19:31
Operator : SY/MD
Sample : J4695-03DL 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

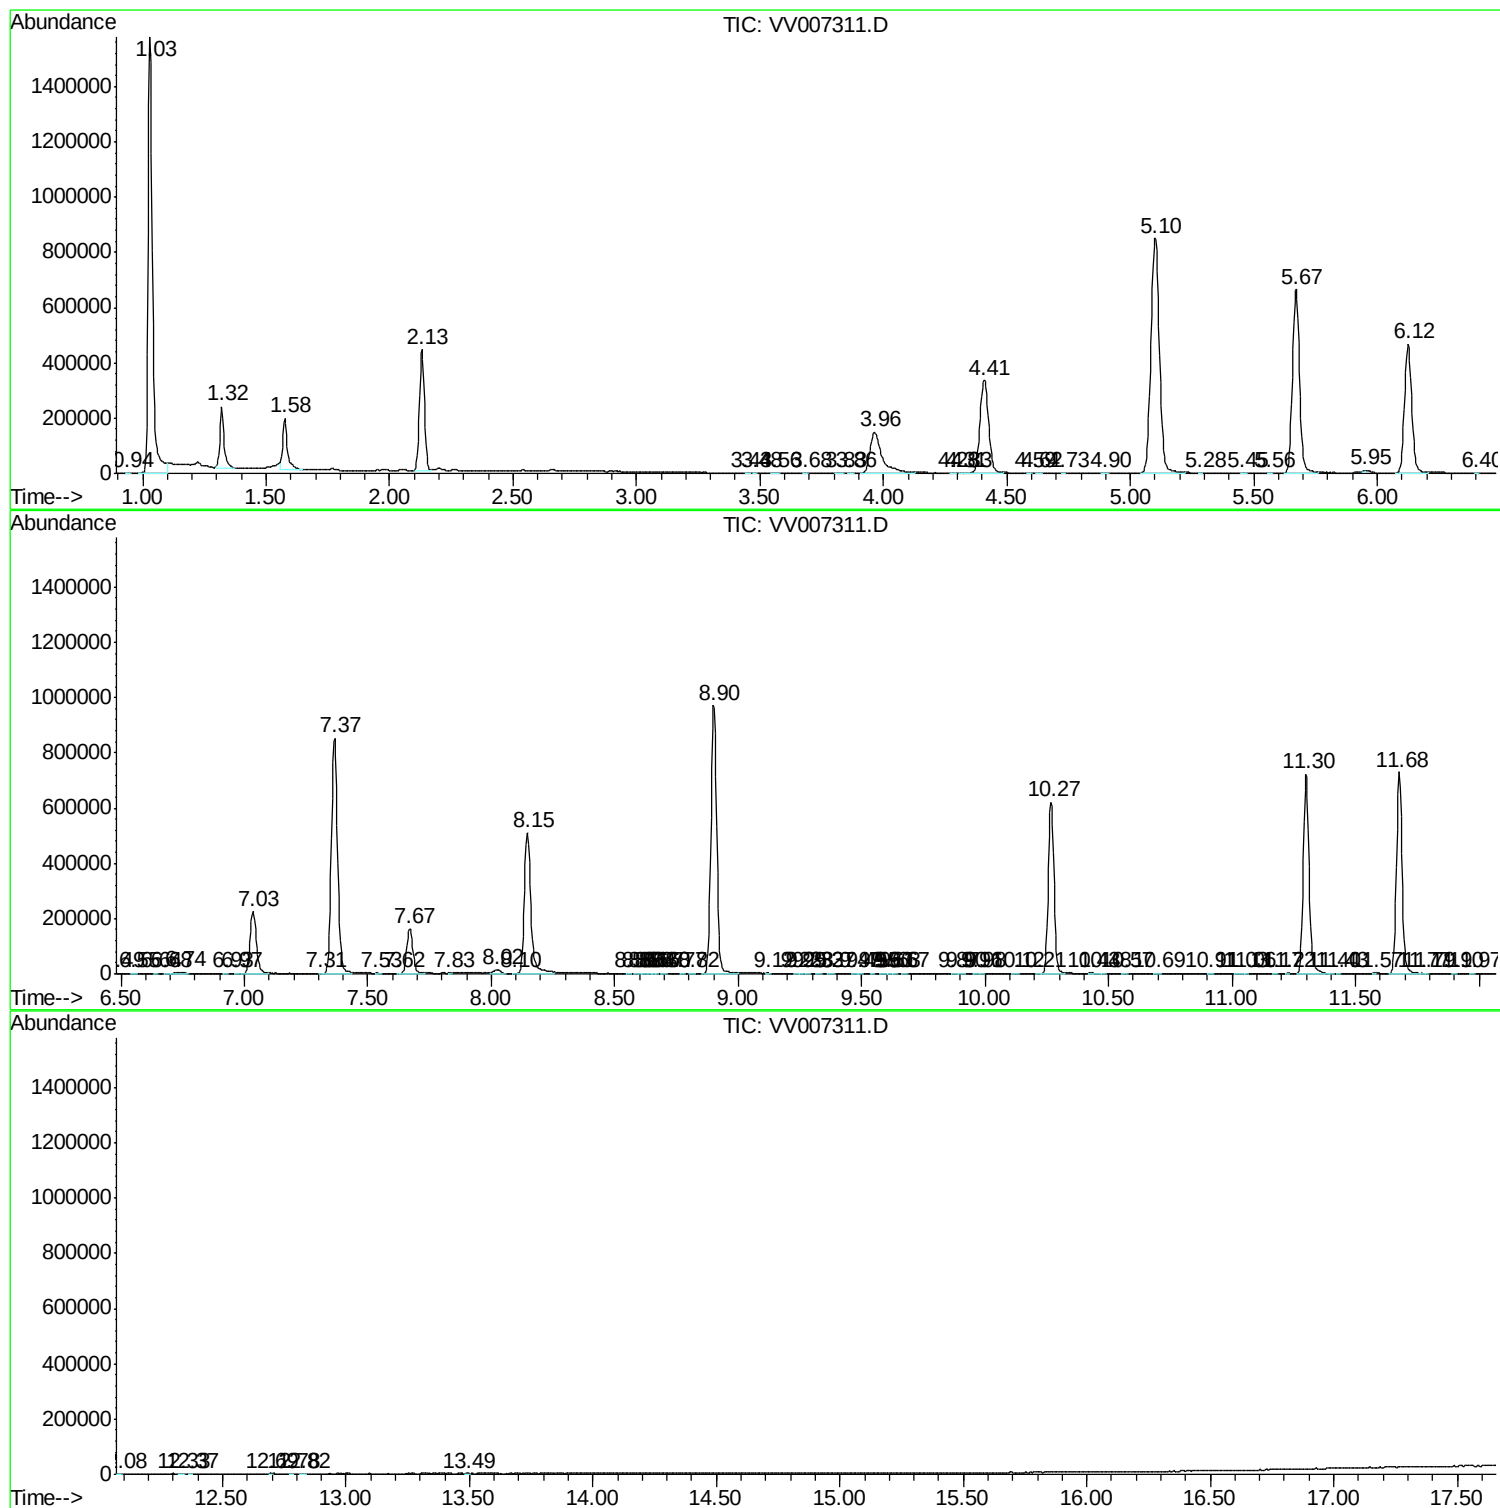

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007311.D
Acq On : 31 Aug 2018 19:31
Operator : SY/MD
Sample : J4695-03DL 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007311.D
Acq On : 31 Aug 2018 19:31
Operator : SY/MD
Sample : J4695-03DL 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc