

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007321.D
 Acq On : 01 Sep 2018 00:02
 Operator : SY/MD
 Sample : J4695-05 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.916	5	8	12	rBV2	478	434	0.002%	0.0002%
2	1.029	29	43	63	rBV	1431513	1785240	82.76%	10.189%
3	1.321	128	134	153	rVB	261092	310548	14.40%	1.772%
4	1.578	208	214	227	rVB	201084	220125	10.20%	1.256%
5	2.131	376	386	398	rBV	501966	701186	32.50%	4.002%
6	3.402	779	781	783	rBV	430	226	0.01%	0.0001%
7	3.414	783	785	788	rVV2	595	465	0.02%	0.0003%
8	3.450	792	796	799	rBV2	611	423	0.02%	0.0002%
9	3.639	852	855	859	rVB2	375	285	0.01%	0.0002%
10	3.839	912	917	919	rBV3	452	447	0.02%	0.0003%
11	3.967	939	957	1008	rBV2	145593	515310	23.89%	2.941%
12	4.408	1075	1094	1118	rBV	353524	848850	39.35%	4.845%
13	4.614	1153	1158	1162	rBV4	685	913	0.04%	0.0005%
14	4.662	1169	1173	1176	rBV2	610	511	0.02%	0.0003%
15	4.697	1182	1184	1186	rBV2	495	266	0.01%	0.0002%
16	4.710	1186	1188	1192	rVB	392	234	0.01%	0.0001%
17	4.742	1192	1198	1201	rBV3	671	656	0.03%	0.0004%
18	4.955	1261	1264	1269	rBV3	579	447	0.02%	0.0003%
19	5.102	1290	1310	1351	rBV2	895658	2157250	100.00%	12.312%
20	5.389	1397	1399	1402	rVB3	436	257	0.01%	0.0001%
21	5.408	1402	1405	1411	rBV4	441	565	0.03%	0.0003%
22	5.434	1411	1413	1414	rVV2	420	234	0.01%	0.0001%
23	5.450	1414	1418	1423	rVV3	1278	1255	0.06%	0.0007%
24	5.472	1423	1425	1429	rVB2	713	417	0.02%	0.0002%
25	5.524	1436	1441	1446	rVB4	762	789	0.04%	0.0005%
26	5.549	1446	1449	1451	rBV	428	315	0.01%	0.0002%
27	5.582	1455	1459	1462	rBV3	445	310	0.01%	0.0002%
28	5.672	1470	1487	1517	rBV	707514	1417278	65.70%	8.089%
29	5.954	1564	1575	1590	rVB8	11102	24025	1.11%	0.137%
30	6.061	1605	1608	1610	rBV4	495	319	0.01%	0.0002%
31	6.125	1613	1628	1656	rBV	498975	1004677	46.57%	5.734%
32	6.347	1693	1697	1699	rBV4	391	311	0.01%	0.0002%
33	6.421	1716	1720	1722	rBV3	266	252	0.01%	0.0001%
34	6.456	1728	1731	1734	rBV2	323	246	0.01%	0.0001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007321.D
 Acq On : 01 Sep 2018 00:02
 Operator : SY/MD
 Sample : J4695-05 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.508	1745	1747	1751	rBV3	365	309	0.01%	0.002%
36	6.527	1751	1753	1757	rVB3	573	392	0.02%	0.002%
37	6.546	1757	1759	1763	rBV2	331	250	0.01%	0.001%
38	6.639	1783	1788	1790	rBV3	767	663	0.03%	0.004%
39	6.739	1808	1819	1821	rBV5	3145	4249	0.20%	0.024%
40	6.810	1839	1841	1844	rVB2	461	261	0.01%	0.001%
41	6.829	1844	1847	1850	rVB2	467	343	0.02%	0.002%
42	6.861	1853	1857	1862	rBV3	431	536	0.02%	0.003%
43	6.909	1869	1872	1875	rBV3	434	337	0.02%	0.002%
44	6.948	1881	1884	1886	rBV3	352	244	0.01%	0.001%
45	7.035	1898	1911	1933	rBV	232034	418787	19.41%	2.390%
46	7.205	1962	1964	1967	rBV2	486	250	0.01%	0.001%
47	7.366	2000	2014	2043	rBV	914270	1605008	74.40%	9.160%
48	7.578	2078	2080	2084	rBV2	500	297	0.01%	0.002%
49	7.598	2084	2086	2089	rBV3	481	273	0.01%	0.002%
50	7.671	2096	2109	2124	rBV	168712	292317	13.55%	1.668%
51	8.022	2210	2218	2231	rVB4	8611	15870	0.74%	0.091%
52	8.089	2236	2239	2243	rBV3	614	484	0.02%	0.003%
53	8.147	2243	2257	2288	rBV2	499087	936188	43.40%	5.343%
54	8.569	2384	2388	2391	rBV3	344	324	0.02%	0.002%
55	8.810	2458	2463	2466	rBV4	731	628	0.03%	0.004%
56	8.832	2466	2470	2472	rBV2	518	281	0.01%	0.002%
57	8.848	2472	2475	2478	rBV2	497	383	0.02%	0.002%
58	8.900	2478	2491	2516	rBV	1028572	1677306	77.75%	9.573%
59	9.176	2571	2577	2579	rBV5	1085	1153	0.05%	0.007%
60	9.247	2595	2599	2600	rBV2	428	271	0.01%	0.002%
61	9.276	2605	2608	2612	rBV3	491	459	0.02%	0.003%
62	9.340	2624	2628	2630	rBV	481	379	0.02%	0.002%
63	9.366	2634	2636	2639	rBV2	506	301	0.01%	0.002%
64	9.443	2656	2660	2662	rBV2	541	368	0.02%	0.002%
65	9.459	2662	2665	2671	rVB4	403	351	0.02%	0.002%
66	9.514	2679	2682	2686	rBV2	375	361	0.02%	0.002%
67	9.610	2710	2712	2718	rVB2	558	509	0.02%	0.003%
68	9.639	2718	2721	2724	rBV3	398	352	0.02%	0.002%
69	9.745	2749	2754	2756	rBV3	535	447	0.02%	0.003%
70	9.858	2785	2789	2792	rBV2	394	313	0.01%	0.002%
71	9.932	2808	2812	2813	rBV2	321	230	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007321.D
 Acq On : 01 Sep 2018 00:02
 Operator : SY/MD
 Sample : J4695-05 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	10.057	2849	2851	2854	rBV2	491	339	0.02%	0.002%
73	10.128	2870	2873	2875	rBV3	660	509	0.02%	0.003%
74	10.170	2883	2886	2888	rBV2	329	237	0.01%	0.001%
75	10.266	2903	2916	2938	rBV	644317	1026369	47.58%	5.858%
76	10.430	2960	2967	2978	rVB4	1607	2395	0.11%	0.014%
77	10.475	2978	2981	2984	rBV3	390	283	0.01%	0.002%
78	10.610	3021	3023	3027	rVB2	457	274	0.01%	0.002%
79	10.832	3087	3092	3094	rBV2	426	366	0.02%	0.002%
80	10.874	3102	3105	3107	rBV3	447	309	0.01%	0.002%
81	10.938	3122	3125	3130	rBV2	415	456	0.02%	0.003%
82	11.060	3159	3163	3167	rBV4	477	466	0.02%	0.003%
83	11.160	3192	3194	3197	rVB2	355	230	0.01%	0.001%
84	11.202	3205	3207	3211	rBV2	464	284	0.01%	0.002%
85	11.231	3213	3216	3219	rBV3	966	735	0.03%	0.004%
86	11.302	3225	3238	3266	rBV	769119	1242126	57.58%	7.089%
87	11.530	3307	3309	3312	rVB2	497	299	0.01%	0.002%
88	11.584	3320	3326	3331	rBV5	1512	2054	0.10%	0.012%
89	11.678	3342	3355	3378	rBV	785860	1266341	58.70%	7.227%
90	11.896	3420	3423	3426	rBV2	545	440	0.02%	0.003%
91	12.285	3541	3544	3546	rBV4	492	271	0.01%	0.002%
92	12.446	3592	3594	3597	rVB2	640	339	0.02%	0.002%
93	12.591	3636	3639	3640	rBV2	651	321	0.01%	0.002%
94	12.732	3680	3683	3685	rBV3	625	477	0.02%	0.003%
95	13.025	3773	3774	3776	rBV2	422	223	0.01%	0.001%
96	13.552	3934	3938	3939	rBV2	1087	831	0.04%	0.005%
97	13.716	3987	3989	3991	rBV3	647	290	0.01%	0.002%
98	14.063	4095	4097	4099	rBV3	841	419	0.02%	0.002%
99	14.568	4252	4254	4257	rBV4	1122	681	0.03%	0.004%
100	17.272	5092	5095	5099	rBV	30379	16488	0.76%	0.094%


Sum of corrected areas: 17521392

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007321.D
Acq On : 01 Sep 2018 00:02
Operator : SY/MD
Sample : J4695-05 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

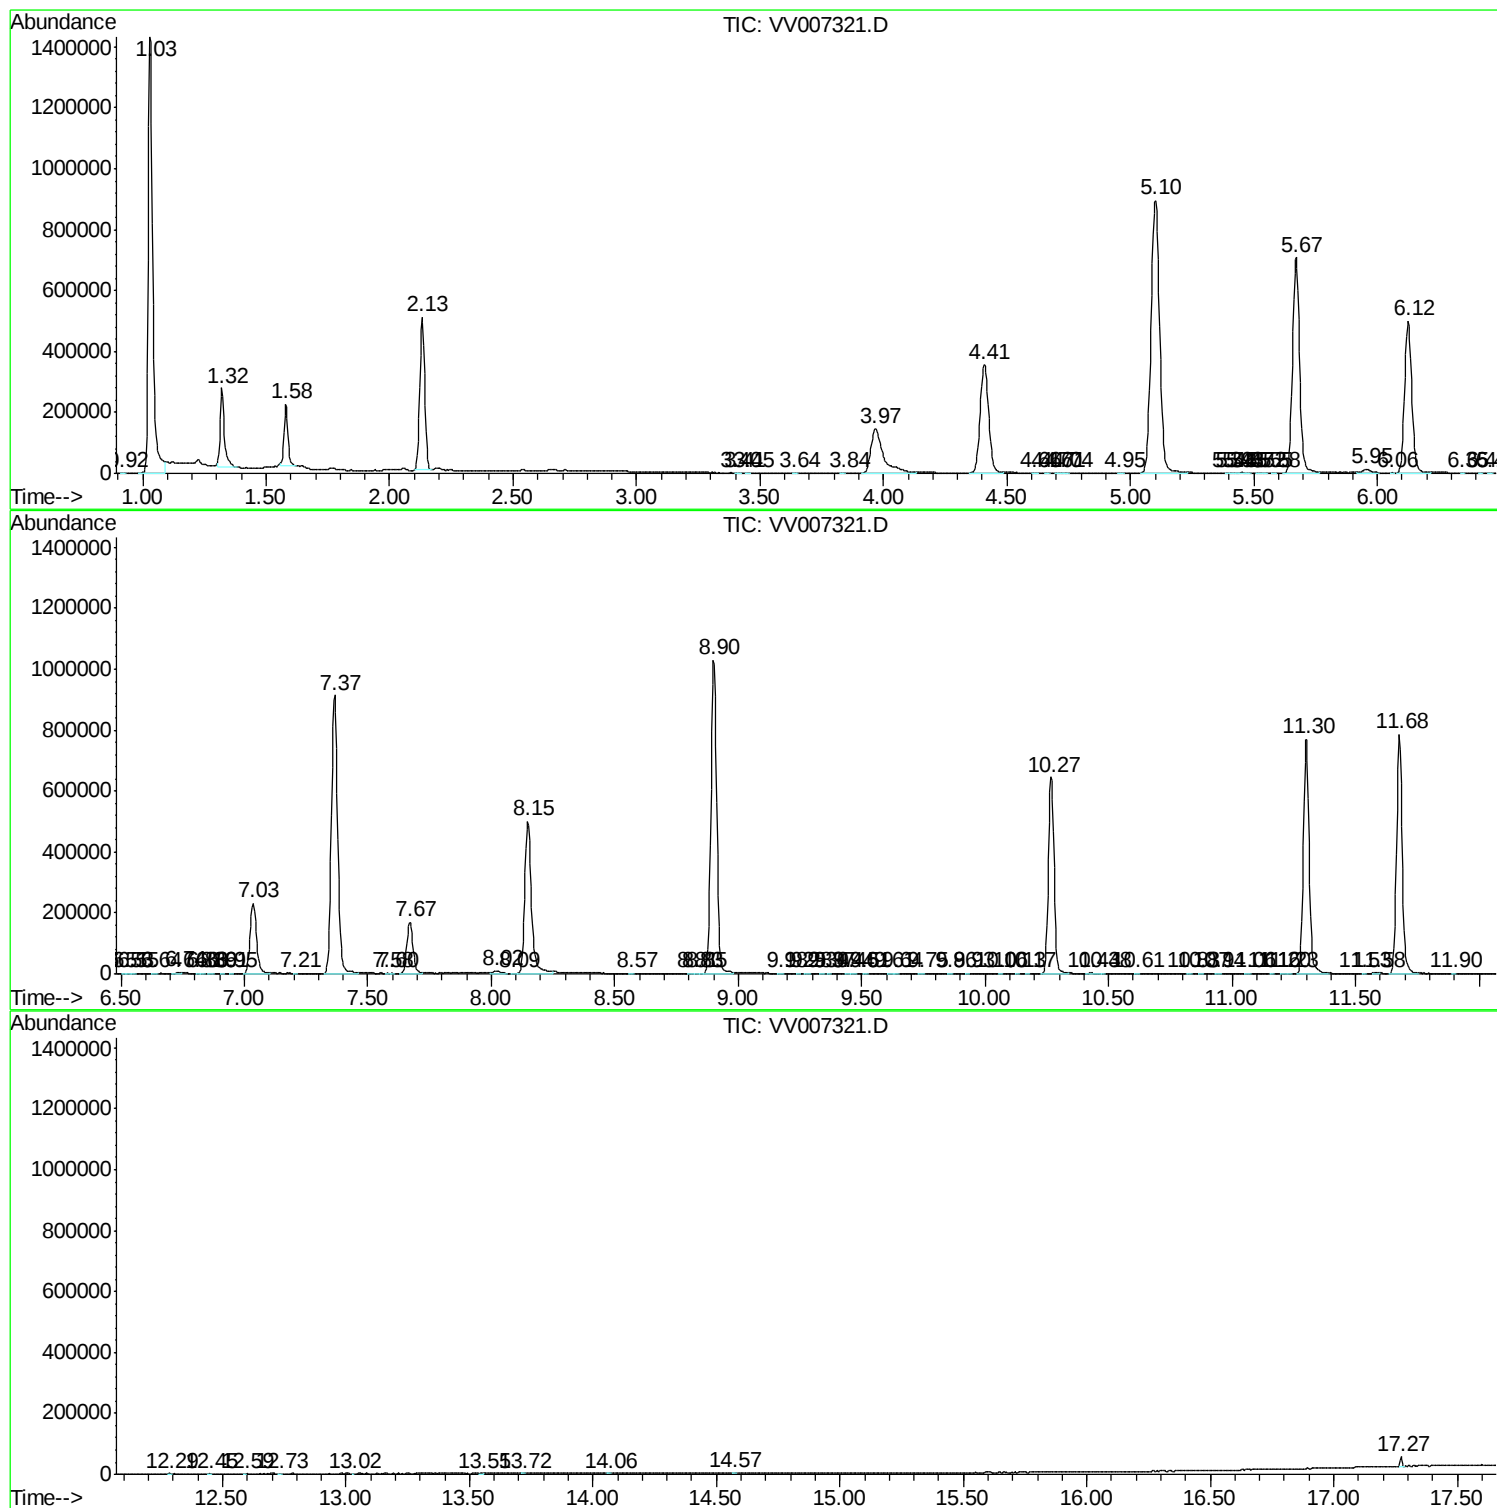

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007321.D
Acq On : 01 Sep 2018 00:02
Operator : SY/MD
Sample : J4695-05 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007321.D
Acq On : 01 Sep 2018 00:02
Operator : SY/MD
Sample : J4695-05 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc