

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007324.D
 Acq On : 01 Sep 2018 01:15
 Operator : SY/MD
 Sample : J4695-08 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	14	17	22	rVB3	414	376	0.002%	0.0002%
2	1.029	26	43	68	rBV	1518370	1874024	88.67%	10.893%
3	1.321	127	134	154	rVB	263601	312207	14.77%	1.815%
4	1.582	209	215	227	rVB	201339	224601	10.63%	1.306%
5	2.132	376	386	398	rBV	487134	683607	32.35%	3.974%
6	3.241	729	731	733	rBV2	631	276	0.01%	0.0002%
7	3.337	759	761	764	rBV3	562	304	0.01%	0.0002%
8	3.482	800	806	809	rVV3	641	663	0.03%	0.0004%
9	3.611	842	846	849	rBV2	527	381	0.02%	0.0002%
10	3.707	873	876	878	rBV	440	259	0.01%	0.0002%
11	3.752	887	890	892	rBV3	452	297	0.01%	0.0002%
12	3.800	903	905	908	rVB3	452	240	0.01%	0.0001%
13	3.868	922	926	928	rBV	621	429	0.02%	0.0002%
14	3.971	938	958	979	rBV	132442	444808	21.05%	2.586%
15	4.228	1035	1038	1043	rVB4	776	609	0.03%	0.0004%
16	4.305	1060	1062	1067	rBV3	379	323	0.02%	0.0002%
17	4.408	1075	1094	1117	rBV	349595	835697	39.54%	4.858%
18	4.630	1160	1163	1166	rVB2	437	237	0.01%	0.0001%
19	4.800	1211	1216	1217	rBV	388	300	0.01%	0.0002%
20	4.890	1239	1244	1246	rBV2	421	386	0.02%	0.0002%
21	4.938	1257	1259	1264	rVB2	288	245	0.01%	0.0001%
22	5.102	1290	1310	1349	rBV2	879875	2113439	100.00%	12.285%
23	5.344	1381	1385	1389	rBV4	539	450	0.02%	0.0003%
24	5.446	1412	1417	1425	rVB4	988	1255	0.06%	0.0007%
25	5.520	1437	1440	1443	rBV4	400	273	0.01%	0.0002%
26	5.553	1447	1450	1455	rVB3	541	415	0.02%	0.0002%
27	5.672	1471	1487	1517	rBV	697497	1388939	65.72%	8.073%
28	5.951	1564	1574	1587	rVB6	8534	18212	0.86%	0.106%
29	6.009	1587	1592	1596	rVB5	597	625	0.03%	0.0004%
30	6.041	1596	1602	1603	rBV5	646	580	0.03%	0.0003%
31	6.125	1612	1628	1655	rBV	491300	987730	46.74%	5.741%
32	6.247	1662	1666	1675	rVB7	2005	2890	0.14%	0.0017%
33	6.450	1727	1729	1733	rVB2	526	333	0.02%	0.0002%
34	6.472	1733	1736	1738	rVB2	502	257	0.01%	0.0001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007324.D
 Acq On : 01 Sep 2018 01:15
 Operator : SY/MD
 Sample : J4695-08 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.495	1738	1743	1744	rBV2	543	338	0.02%	0.002%
36	6.588	1769	1772	1774	rVV	353	241	0.01%	0.001%
37	6.643	1782	1789	1793	rBV4	789	1098	0.05%	0.006%
38	6.742	1812	1820	1825	rBV5	2121	3582	0.17%	0.021%
39	6.816	1840	1843	1845	rVB2	771	433	0.02%	0.003%
40	6.832	1845	1848	1852	rBV2	559	460	0.02%	0.003%
41	6.903	1867	1870	1876	rBV3	497	448	0.02%	0.003%
42	6.932	1876	1879	1882	rBV2	438	375	0.02%	0.002%
43	7.035	1898	1911	1933	rBV	222906	404909	19.16%	2.354%
44	7.292	1988	1991	1997	rVB4	650	517	0.02%	0.003%
45	7.366	1997	2014	2034	rBV	891633	1557142	73.68%	9.051%
46	7.530	2063	2065	2070	rVB3	614	298	0.01%	0.002%
47	7.623	2090	2094	2096	rBV4	834	715	0.03%	0.004%
48	7.668	2097	2108	2133	rVV	160331	277832	13.15%	1.615%
49	8.025	2214	2219	2225	rVB4	2371	2935	0.14%	0.017%
50	8.147	2242	2257	2285	rBV2	497718	942206	44.58%	5.477%
51	8.482	2357	2361	2364	rVB5	745	512	0.02%	0.003%
52	8.552	2381	2383	2387	rVB4	460	255	0.01%	0.001%
53	8.639	2408	2410	2415	rVV3	679	493	0.02%	0.003%
54	8.662	2415	2417	2420	rVB3	412	254	0.01%	0.001%
55	8.681	2420	2423	2425	rVB	435	239	0.01%	0.001%
56	8.758	2438	2447	2450	rVB3	445	660	0.03%	0.004%
57	8.800	2457	2460	2461	rBV	679	341	0.02%	0.002%
58	8.848	2472	2475	2477	rBV3	551	333	0.02%	0.002%
59	8.900	2477	2491	2511	rBV	1004112	1645463	77.86%	9.565%
60	9.189	2578	2581	2586	rVV3	678	481	0.02%	0.003%
61	9.215	2586	2589	2594	rVB4	664	537	0.03%	0.003%
62	9.260	2599	2603	2605	rBV2	367	307	0.01%	0.002%
63	9.279	2605	2609	2612	rVB3	354	242	0.01%	0.001%
64	9.311	2616	2619	2622	rBV2	637	373	0.02%	0.002%
65	9.337	2626	2627	2634	rVB3	515	296	0.01%	0.002%
66	9.372	2634	2638	2640	rBV3	540	333	0.02%	0.002%
67	9.417	2649	2652	2655	rBV	397	239	0.01%	0.001%
68	9.469	2664	2668	2673	rVB4	459	445	0.02%	0.003%
69	9.543	2689	2691	2699	rVB4	654	642	0.03%	0.004%
70	9.588	2699	2705	2711	rBV4	629	939	0.04%	0.005%
71	9.684	2731	2735	2738	rBV4	435	395	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007324.D
 Acq On : 01 Sep 2018 01:15
 Operator : SY/MD
 Sample : J4695-08 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	9.794	2767	2769	2774	rVB3	502	420	0.02%	0.002%
73	9.861	2788	2790	2794	rBV3	317	256	0.01%	0.001%
74	10.012	2833	2837	2843	rVB3	670	774	0.04%	0.004%
75	10.041	2843	2846	2851	rBV4	576	610	0.03%	0.004%
76	10.070	2851	2855	2860	rVB3	472	442	0.02%	0.003%
77	10.099	2860	2864	2867	rBV2	482	319	0.02%	0.002%
78	10.150	2877	2880	2882	rVV2	433	287	0.01%	0.002%
79	10.266	2903	2916	2946	rBV	634518	1012380	47.90%	5.885%
80	10.404	2955	2959	2960	rBV	410	313	0.01%	0.002%
81	10.427	2963	2966	2973	rVB3	836	932	0.04%	0.005%
82	10.507	2987	2991	2993	rBV2	382	334	0.02%	0.002%
83	10.620	3017	3026	3029	rBV4	642	857	0.04%	0.005%
84	10.694	3044	3049	3051	rBV2	428	477	0.02%	0.003%
85	10.845	3090	3096	3101	rBV4	654	829	0.04%	0.005%
86	10.913	3113	3117	3122	rVB3	594	590	0.03%	0.003%
87	11.048	3155	3159	3163	rBV3	375	371	0.02%	0.002%
88	11.163	3192	3195	3198	rVB	423	269	0.01%	0.002%
89	11.237	3216	3218	3220	rVB	538	265	0.01%	0.002%
90	11.298	3225	3237	3266	rBV	760327	1211622	57.33%	7.043%
91	11.449	3282	3284	3286	rBV2	383	247	0.01%	0.001%
92	11.678	3341	3355	3382	rVV	760101	1223623	57.90%	7.113%
93	11.806	3393	3395	3398	rBV	378	283	0.01%	0.002%
94	11.906	3423	3426	3433	rBV4	503	589	0.03%	0.003%
95	12.218	3519	3523	3528	rBV4	714	756	0.04%	0.004%
96	12.263	3534	3537	3542	rBV3	660	665	0.03%	0.004%
97	12.285	3542	3544	3555	rVV5	783	1059	0.05%	0.006%
98	12.443	3590	3593	3596	rBV4	486	339	0.02%	0.002%
99	12.726	3678	3681	3685	rBV3	444	361	0.02%	0.002%
100	13.096	3793	3796	3798	rBV3	758	486	0.02%	0.003%


Sum of corrected areas: 17203730

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007324.D
Acq On : 01 Sep 2018 01:15
Operator : SY/MD
Sample : J4695-08 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

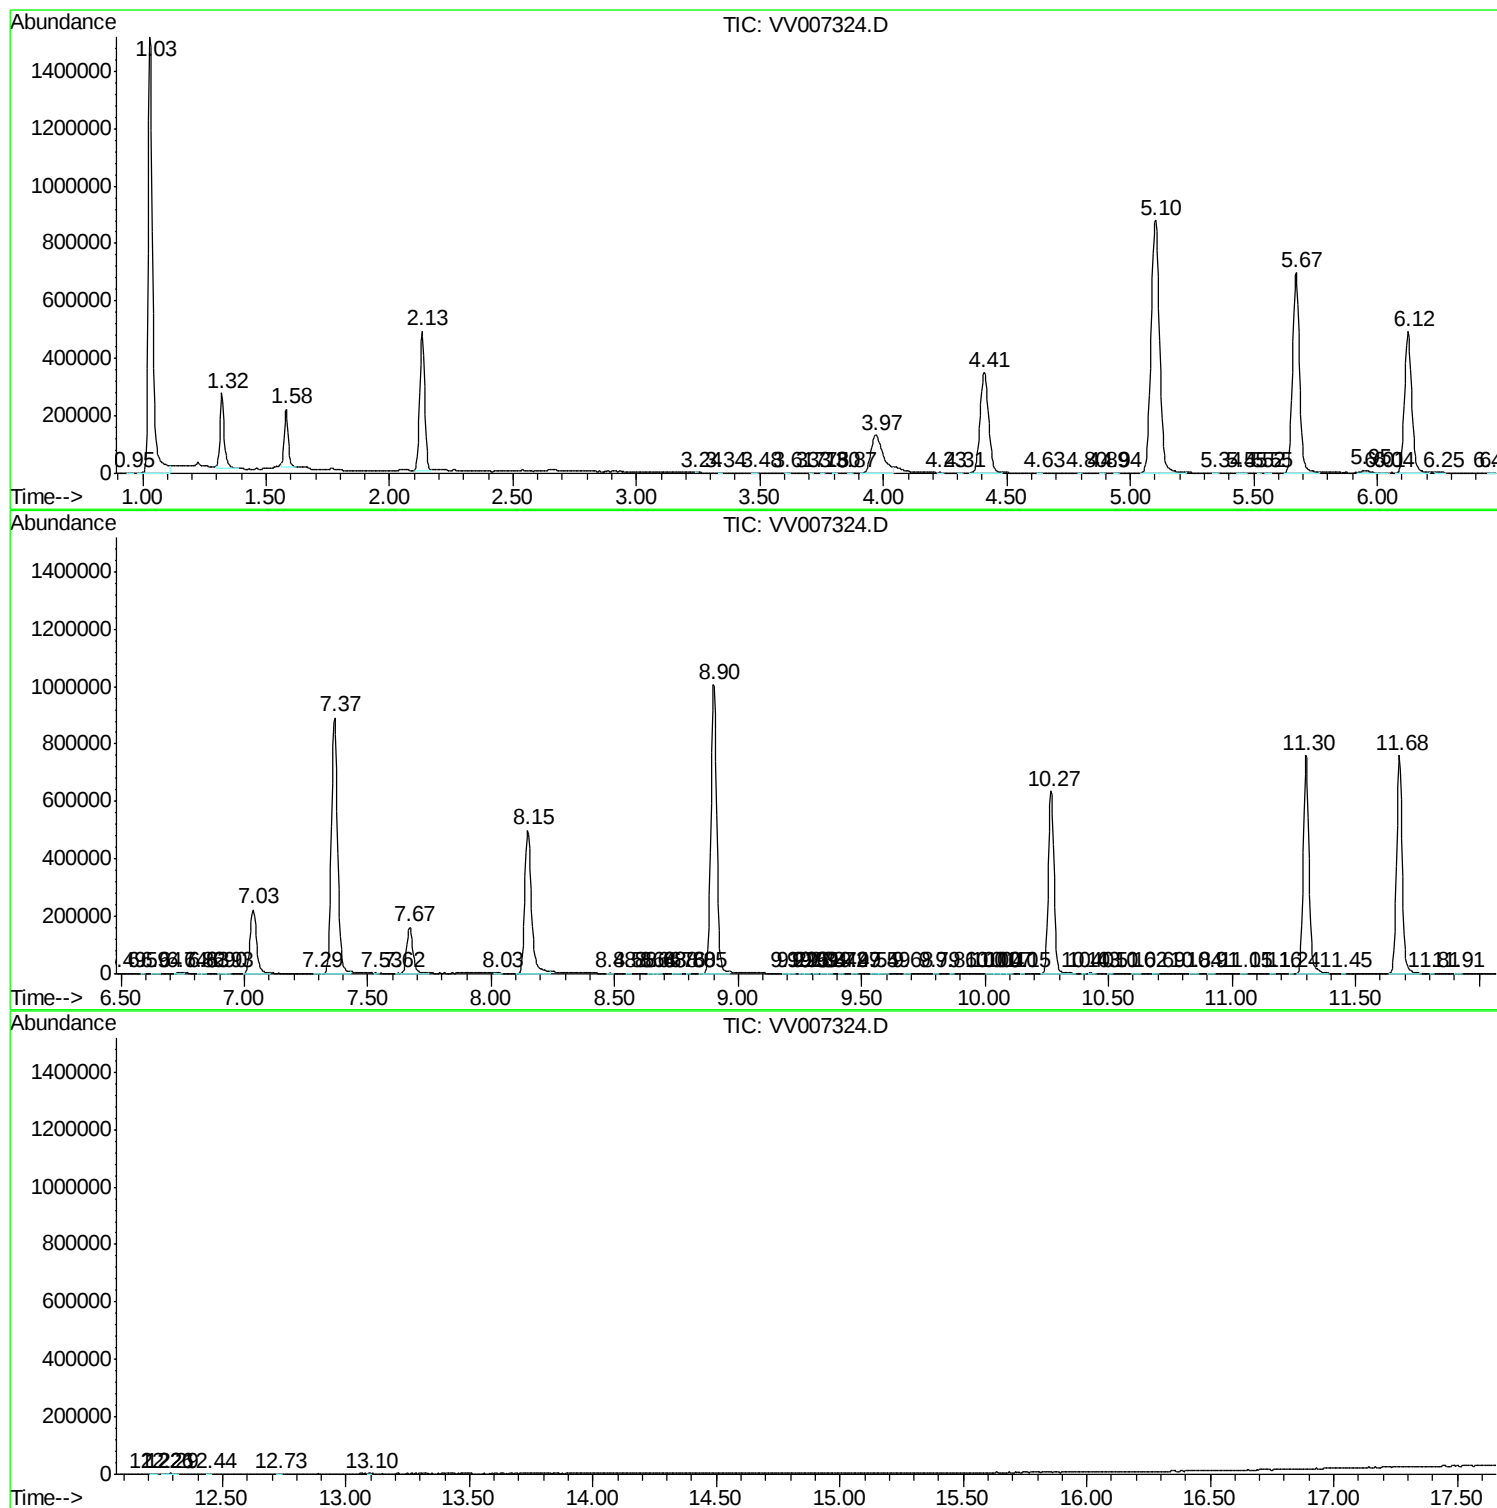

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007324.D
Acq On : 01 Sep 2018 01:15
Operator : SY/MD
Sample : J4695-08 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007324.D
Acq On : 01 Sep 2018 01:15
Operator : SY/MD
Sample : J4695-08 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc