

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007326.D
 Acq On : 01 Sep 2018 02:05
 Operator : SY/MD
 Sample : J4695-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.028	29	43	68	rBV	1438041	1822689	82.84%	10.304%
2	1.321	127	134	153	rVB	265848	307707	13.98%	1.740%
3	1.578	208	214	239	rVB	217285	270550	12.30%	1.529%
4	2.131	376	386	398	rBV	512451	724062	32.91%	4.093%
5	3.289	744	746	748	rBV2	476	248	0.01%	0.001%
6	3.601	841	843	846	rVB2	408	254	0.01%	0.001%
7	3.700	871	874	877	rVB3	497	320	0.01%	0.002%
8	3.726	877	882	885	rBV4	313	265	0.01%	0.001%
9	3.967	938	957	997	rBV	144831	518895	23.58%	2.933%
10	4.295	1055	1059	1061	rBV4	547	427	0.02%	0.002%
11	4.334	1067	1071	1074	rVB4	603	507	0.02%	0.003%
12	4.408	1075	1094	1119	rBV	363879	869245	39.50%	4.914%
13	4.540	1132	1135	1140	rVB3	760	683	0.03%	0.004%
14	4.646	1165	1168	1173	rBV3	420	284	0.01%	0.002%
15	4.774	1206	1208	1210	rBV4	441	248	0.01%	0.001%
16	4.806	1216	1218	1221	rVB2	512	228	0.01%	0.001%
17	4.832	1221	1226	1229	rVB3	624	610	0.03%	0.003%
18	4.868	1234	1237	1239	rBV2	409	258	0.01%	0.001%
19	4.884	1239	1242	1248	rVB2	756	612	0.03%	0.003%
20	4.925	1253	1255	1259	rBV2	381	234	0.01%	0.001%
21	5.012	1278	1282	1285	rBV2	342	250	0.01%	0.001%
22	5.035	1285	1289	1290	rBV3	352	244	0.01%	0.001%
23	5.102	1290	1310	1348	rBV2	915811	2200359	100.00%	12.439%
24	5.292	1367	1369	1373	rVB3	453	259	0.01%	0.001%
25	5.334	1380	1382	1386	rVB	436	253	0.01%	0.001%
26	5.388	1396	1399	1402	rBV3	507	341	0.02%	0.002%
27	5.450	1411	1418	1425	rBV4	938	1445	0.07%	0.008%
28	5.507	1433	1436	1438	rBV3	422	228	0.01%	0.001%
29	5.530	1438	1443	1444	rBV3	297	242	0.01%	0.001%
30	5.578	1457	1458	1462	rVB2	482	257	0.01%	0.001%
31	5.610	1462	1468	1471	rBV3	627	569	0.03%	0.003%
32	5.671	1471	1487	1525	rBV	683960	1383843	62.89%	7.823%
33	5.954	1565	1575	1586	rVB6	9142	17504	0.80%	0.099%
34	6.051	1603	1605	1611	rVB3	517	335	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007326.D
 Acq On : 01 Sep 2018 02:05
 Operator : SY/MD
 Sample : J4695-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.125	1611	1628	1652	rBV	506614	1022560	46.47%	5.781%
36	6.292	1678	1680	1683	rVB3	713	354	0.02%	0.002%
37	6.491	1738	1742	1746	rBV2	496	468	0.02%	0.003%
38	6.530	1750	1754	1760	rBV5	718	792	0.04%	0.004%
39	6.556	1760	1762	1767	rBV2	359	285	0.01%	0.002%
40	6.626	1782	1784	1791	rVV6	524	478	0.02%	0.003%
41	6.655	1791	1793	1796	rVV4	418	287	0.01%	0.002%
42	6.671	1796	1798	1805	rVB4	1046	974	0.04%	0.006%
43	6.707	1805	1809	1810	rBV	719	471	0.02%	0.003%
44	6.803	1837	1839	1844	rVB2	662	581	0.03%	0.003%
45	6.829	1844	1847	1848	rBV	350	233	0.01%	0.001%
46	6.877	1859	1862	1868	rVB3	782	521	0.02%	0.003%
47	6.970	1889	1891	1895	rBV2	511	316	0.01%	0.002%
48	7.035	1898	1911	1934	rBV	231067	420935	19.13%	2.380%
49	7.305	1993	1995	1999	rVB2	501	368	0.02%	0.002%
50	7.366	1999	2014	2047	rBV	933401	1641488	74.60%	9.280%
51	7.668	2096	2108	2129	rBV2	168436	293911	13.36%	1.662%
52	8.022	2210	2218	2227	rVB4	8423	13329	0.61%	0.075%
53	8.147	2244	2257	2294	rBV2	523668	987832	44.89%	5.584%
54	8.469	2353	2357	2361	rBV3	538	466	0.02%	0.003%
55	8.559	2382	2385	2386	rBV2	507	311	0.01%	0.002%
56	8.597	2394	2397	2400	rBV2	726	544	0.02%	0.003%
57	8.668	2417	2419	2422	rVB2	827	413	0.02%	0.002%
58	8.707	2429	2431	2435	rBV4	308	237	0.01%	0.001%
59	8.761	2444	2448	2451	rBV3	605	487	0.02%	0.003%
60	8.777	2451	2453	2456	rVB2	411	231	0.01%	0.001%
61	8.800	2457	2460	2464	rBV2	589	454	0.02%	0.003%
62	8.900	2477	2491	2520	rBV	1007977	1643098	74.67%	9.289%
63	9.189	2578	2581	2588	rVB3	1241	1308	0.06%	0.007%
64	9.234	2590	2595	2596	rBV3	498	314	0.01%	0.002%
65	9.308	2611	2618	2621	rBV2	470	617	0.03%	0.003%
66	9.430	2652	2656	2661	rVB3	659	678	0.03%	0.004%
67	9.523	2682	2685	2687	rBV2	389	277	0.01%	0.002%
68	9.575	2697	2701	2703	rBV2	513	457	0.02%	0.003%
69	9.758	2754	2758	2762	rVB2	523	371	0.02%	0.002%
70	9.781	2762	2765	2768	rBV2	398	285	0.01%	0.002%
71	9.800	2768	2771	2776	rVB3	543	443	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007326.D
 Acq On : 01 Sep 2018 02:05
 Operator : SY/MD
 Sample : J4695-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	9.842	2781	2784	2787	rVB3	536	326	0.01%	0.002%
73	9.864	2787	2791	2792	rBV2	347	246	0.01%	0.001%
74	9.954	2817	2819	2823	rBV2	359	230	0.01%	0.001%
75	9.973	2823	2825	2831	rVB2	424	278	0.01%	0.002%
76	10.047	2843	2848	2850	rBV2	362	363	0.02%	0.002%
77	10.121	2868	2871	2873	rBV2	376	235	0.01%	0.001%
78	10.179	2884	2889	2890	rBV	489	406	0.02%	0.002%
79	10.266	2902	2916	2935	rBV	653222	1038713	47.21%	5.872%
80	10.469	2976	2979	2987	rVB4	508	542	0.02%	0.003%
81	10.649	3033	3035	3040	rVB3	638	472	0.02%	0.003%
82	10.678	3040	3044	3046	rBV	534	468	0.02%	0.003%
83	10.906	3113	3115	3118	rBV2	582	387	0.02%	0.002%
84	10.954	3126	3130	3132	rBV2	506	329	0.01%	0.002%
85	10.989	3138	3141	3143	rVB2	497	259	0.01%	0.001%
86	11.060	3159	3163	3166	rBV2	398	294	0.01%	0.002%
87	11.105	3172	3177	3179	rBV3	477	518	0.02%	0.003%
88	11.224	3210	3214	3216	rBV3	406	367	0.02%	0.002%
89	11.301	3225	3238	3269	rBV	753712	1202819	54.66%	6.800%
90	11.543	3311	3313	3315	rBV2	511	304	0.01%	0.002%
91	11.678	3342	3355	3380	rBV	799777	1276272	58.00%	7.215%
92	11.935	3432	3435	3437	rBV2	458	351	0.02%	0.002%
93	12.022	3460	3462	3466	rBV2	386	286	0.01%	0.002%
94	12.838	3713	3716	3719	rBV4	708	484	0.02%	0.003%
95	12.864	3721	3724	3726	rBV2	436	307	0.01%	0.002%
96	12.896	3731	3734	3738	rVV3	655	423	0.02%	0.002%
97	13.395	3886	3889	3891	rVB4	763	456	0.02%	0.003%
98	13.407	3891	3893	3898	rBV4	482	383	0.02%	0.002%
99	13.539	3931	3934	3939	rBV4	533	593	0.03%	0.003%
100	13.723	3989	3991	3993	rBV2	616	232	0.01%	0.001%


Sum of corrected areas: 17688972

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007326.D
Acq On : 01 Sep 2018 02:05
Operator : SY/MD
Sample : J4695-12 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE55

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

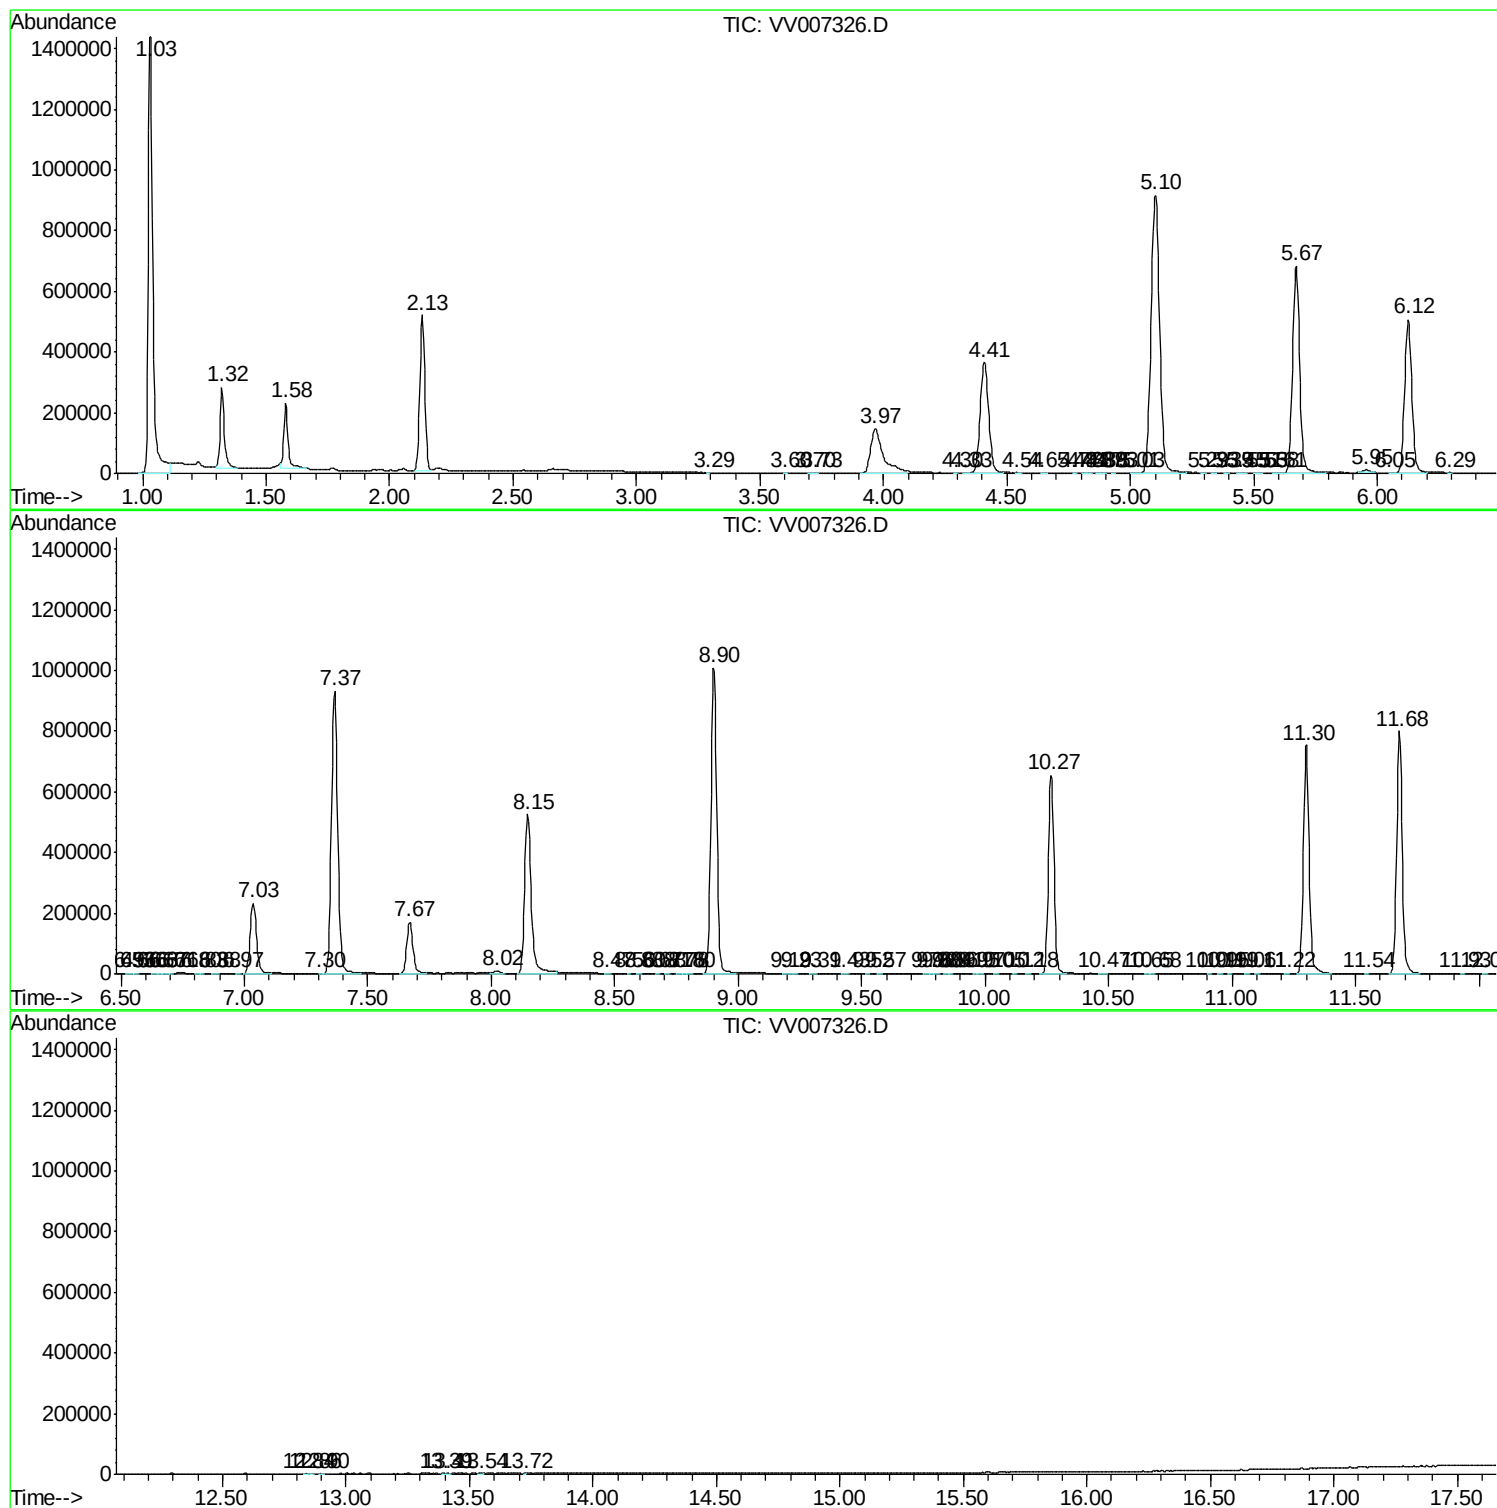

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007326.D
Acq On : 01 Sep 2018 02:05
Operator : SY/MD
Sample : J4695-12 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE55

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007326.D
Acq On : 01 Sep 2018 02:05
Operator : SY/MD
Sample : J4695-12 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE55

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc