

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007327.D
 Acq On : 01 Sep 2018 02:29
 Operator : SY/MD
 Sample : J4695-13 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	13	17	22	rBV3	511	518	0.002%	0.003%
2	1.028	29	43	66	rBV	1424685	1764407	82.76%	10.251%
3	1.321	128	134	152	rVB	257914	294871	13.83%	1.713%
4	1.578	208	214	224	rVB	200423	216038	10.13%	1.255%
5	2.131	376	386	399	rBV	497524	693080	32.51%	4.027%
6	3.453	795	797	800	rVB2	578	310	0.01%	0.002%
7	3.479	802	805	807	rBV2	620	274	0.01%	0.002%
8	3.498	808	811	815	rVV3	342	253	0.01%	0.001%
9	3.585	835	838	842	rVB2	400	245	0.01%	0.001%
10	3.636	852	854	858	rVB3	349	234	0.01%	0.001%
11	3.720	875	880	883	rBV3	376	395	0.02%	0.002%
12	3.855	919	922	925	rBV2	308	234	0.01%	0.001%
13	3.897	929	935	937	rBV2	390	409	0.02%	0.002%
14	3.967	940	957	1010	rBV	137126	496192	23.27%	2.883%
15	4.286	1052	1056	1059	rBV5	579	433	0.02%	0.003%
16	4.408	1075	1094	1124	rBV	348834	841615	39.47%	4.890%
17	4.662	1171	1173	1179	rBV4	567	444	0.02%	0.003%
18	4.739	1194	1197	1201	rBV3	653	617	0.03%	0.004%
19	4.890	1239	1244	1247	rVB3	573	555	0.03%	0.003%
20	4.909	1247	1250	1252	rBV2	441	277	0.01%	0.002%
21	4.948	1259	1262	1265	rVV	406	267	0.01%	0.002%
22	5.102	1291	1310	1349	rBV2	896032	2132041	100.00%	12.387%
23	5.343	1382	1385	1388	rVB2	357	235	0.01%	0.001%
24	5.382	1394	1397	1399	rVV2	347	248	0.01%	0.001%
25	5.478	1425	1427	1431	rVB2	470	257	0.01%	0.001%
26	5.501	1431	1434	1435	rBV	549	230	0.01%	0.001%
27	5.517	1437	1439	1444	rVB2	538	320	0.02%	0.002%
28	5.565	1451	1454	1458	rBV3	396	245	0.01%	0.001%
29	5.671	1467	1487	1527	rBV	695972	1398495	65.59%	8.125%
30	5.951	1564	1574	1588	rVB2	10125	19960	0.94%	0.116%
31	6.003	1588	1590	1592	rBV2	543	308	0.01%	0.002%
32	6.125	1612	1628	1657	rBV	490920	991931	46.52%	5.763%
33	6.305	1680	1684	1689	rVB3	529	562	0.03%	0.003%
34	6.427	1719	1722	1724	rBV	437	331	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007327.D
 Acq On : 01 Sep 2018 02:29
 Operator : SY/MD
 Sample : J4695-13 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.475	1733	1737	1739	rBV3	333	238	0.01%	0.001%
36	6.507	1744	1747	1749	rBV3	396	276	0.01%	0.002%
37	6.559	1761	1763	1769	rVB4	477	266	0.01%	0.002%
38	6.636	1782	1787	1788	rBV	712	469	0.02%	0.003%
39	6.662	1792	1795	1797	rVV2	684	322	0.02%	0.002%
40	6.739	1809	1819	1822	rBV3	2295	3522	0.17%	0.020%
41	6.806	1836	1840	1843	rVV2	543	430	0.02%	0.002%
42	6.938	1877	1881	1886	rBV4	619	613	0.03%	0.004%
43	7.035	1896	1911	1932	rBV	222721	408382	19.15%	2.373%
44	7.186	1955	1958	1962	rVB2	802	600	0.03%	0.003%
45	7.366	1999	2014	2049	rBV	894394	1566772	73.49%	9.103%
46	7.668	2097	2108	2125	rBV	162638	277297	13.01%	1.611%
47	7.787	2142	2145	2151	rVB4	671	691	0.03%	0.004%
48	8.022	2210	2218	2231	rVB5	9825	16708	0.78%	0.097%
49	8.147	2242	2257	2287	rBV2	502859	936461	43.92%	5.441%
50	8.549	2380	2382	2389	rVB4	608	619	0.03%	0.004%
51	8.578	2389	2391	2393	rBV	387	260	0.01%	0.002%
52	8.610	2398	2401	2405	rBV3	374	294	0.01%	0.002%
53	8.639	2407	2410	2414	rVB3	416	331	0.02%	0.002%
54	8.694	2425	2427	2429	rVV2	515	270	0.01%	0.002%
55	8.729	2432	2438	2441	rBV3	565	645	0.03%	0.004%
56	8.768	2447	2450	2454	rVB4	375	243	0.01%	0.001%
57	8.800	2457	2460	2463	rBV2	318	251	0.01%	0.001%
58	8.900	2477	2491	2520	rBV	1020006	1666331	78.16%	9.681%
59	9.176	2572	2577	2581	rVV4	455	594	0.03%	0.003%
60	9.295	2611	2614	2616	rBV3	287	215	0.01%	0.001%
61	9.366	2633	2636	2639	rVB	578	347	0.02%	0.002%
62	9.385	2639	2642	2646	rBV3	447	398	0.02%	0.002%
63	9.465	2662	2667	2670	rBV3	443	373	0.02%	0.002%
64	9.530	2685	2687	2693	rVB3	503	384	0.02%	0.002%
65	9.588	2703	2705	2709	rVB3	363	280	0.01%	0.002%
66	9.623	2713	2716	2719	rBV4	393	276	0.01%	0.002%
67	9.671	2724	2731	2733	rBV3	684	653	0.03%	0.004%
68	9.726	2743	2748	2749	rBV2	278	258	0.01%	0.001%
69	9.790	2764	2768	2772	rBV3	430	386	0.02%	0.002%
70	9.938	2808	2814	2817	rBV2	323	320	0.02%	0.002%
71	10.047	2845	2848	2851	rBV	595	311	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007327.D
 Acq On : 01 Sep 2018 02:29
 Operator : SY/MD
 Sample : J4695-13 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	10.083	2854	2859	2861	rBV2	367	327	0.02%	0.002%
73	10.147	2877	2879	2884	rVB2	498	316	0.01%	0.002%
74	10.186	2888	2891	2895	rBV3	406	365	0.02%	0.002%
75	10.266	2903	2916	2938	rBV	636289	1011267	47.43%	5.875%
76	10.433	2959	2968	2973	rBV4	1510	2004	0.09%	0.012%
77	10.469	2975	2979	2984	rVB3	444	415	0.02%	0.002%
78	10.498	2984	2988	2990	rBV	499	303	0.01%	0.002%
79	10.565	3006	3009	3011	rBV	376	226	0.01%	0.001%
80	10.758	3065	3069	3072	rBV2	289	271	0.01%	0.002%
81	10.780	3072	3076	3080	rVB3	340	312	0.01%	0.002%
82	10.829	3083	3091	3094	rBV4	400	598	0.03%	0.003%
83	10.906	3111	3115	3119	rVV4	1137	869	0.04%	0.005%
84	10.964	3129	3133	3139	rBV2	473	616	0.03%	0.004%
85	11.025	3144	3152	3156	rBV3	700	986	0.05%	0.006%
86	11.073	3163	3167	3170	rBV3	483	399	0.02%	0.002%
87	11.211	3207	3210	3214	rVB3	497	317	0.01%	0.002%
88	11.237	3214	3218	3221	rVB2	664	482	0.02%	0.003%
89	11.301	3224	3238	3265	rBV	759421	1216879	57.08%	7.070%
90	11.446	3281	3283	3286	rVB2	501	272	0.01%	0.002%
91	11.465	3286	3289	3291	rBV2	537	337	0.02%	0.002%
92	11.523	3304	3307	3309	rBV3	386	232	0.01%	0.001%
93	11.678	3342	3355	3379	rBV	765095	1226833	57.54%	7.128%
94	12.089	3478	3483	3486	rBV3	579	626	0.03%	0.004%
95	12.343	3559	3562	3565	rBV3	501	334	0.02%	0.002%
96	12.623	3646	3649	3653	rBV4	540	450	0.02%	0.003%
97	13.308	3859	3862	3864	rBV3	745	491	0.02%	0.003%
98	13.456	3906	3908	3911	rBV2	603	436	0.02%	0.003%
99	13.977	4067	4070	4071	rBV2	613	332	0.02%	0.002%
100	14.436	4211	4213	4217	rBV5	853	691	0.03%	0.004%


Sum of corrected areas: 17211903

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007327.D
Acq On : 01 Sep 2018 02:29
Operator : SY/MD
Sample : J4695-13 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

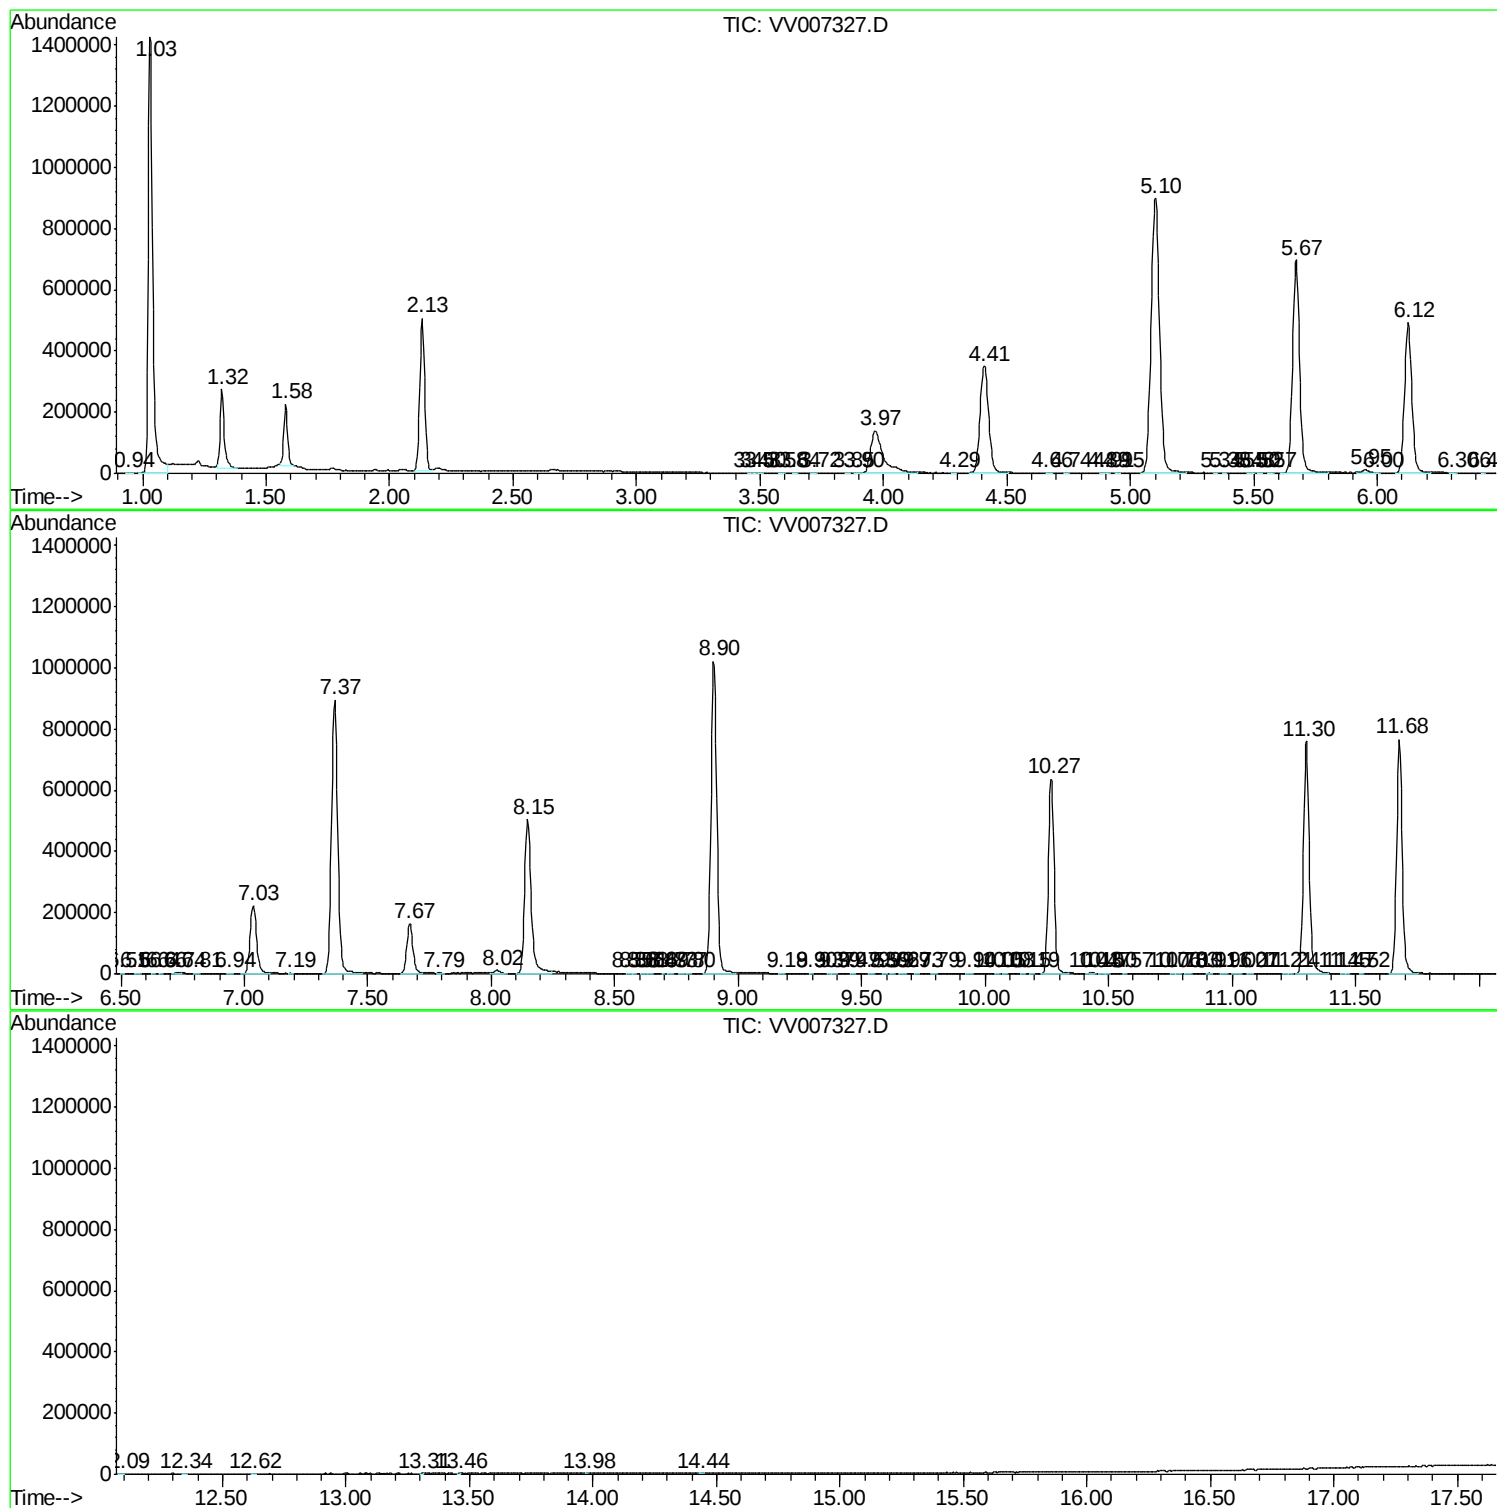

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007327.D
Acq On : 01 Sep 2018 02:29
Operator : SY/MD
Sample : J4695-13 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE56

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007327.D
Acq On : 01 Sep 2018 02:29
Operator : SY/MD
Sample : J4695-13 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
