

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007328.D
 Acq On : 01 Sep 2018 02:54
 Operator : SY/MD
 Sample : J4695-14 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.029	25	43	68	rBV	1399601	1752357	81.93%	10.073%
2	1.321	128	134	157	rVB	258008	308063	14.40%	1.771%
3	1.578	209	214	230	rVB	200160	229802	10.74%	1.321%
4	2.131	376	386	398	rBV	500662	694653	32.48%	3.993%
5	3.347	762	764	767	rBV3	467	235	0.01%	0.001%
6	3.440	790	793	794	rBV2	484	231	0.01%	0.001%
7	3.524	817	819	821	rBV2	469	271	0.01%	0.002%
8	3.643	852	856	859	rVV3	302	247	0.01%	0.001%
9	3.794	899	903	906	rBV3	388	254	0.01%	0.001%
10	3.852	914	921	923	rBV2	426	434	0.02%	0.002%
11	3.893	931	934	936	rBV2	409	315	0.01%	0.002%
12	3.971	939	958	1005	rBV2	137940	498385	23.30%	2.865%
13	4.315	1062	1065	1071	rVB5	889	671	0.03%	0.004%
14	4.408	1074	1094	1125	rBV	354825	856164	40.03%	4.921%
15	4.582	1146	1148	1152	rVB3	511	270	0.01%	0.002%
16	4.643	1165	1167	1172	rVB3	444	335	0.02%	0.002%
17	4.723	1189	1192	1196	rVB	430	359	0.02%	0.002%
18	4.746	1196	1199	1201	rBV2	433	312	0.01%	0.002%
19	4.797	1211	1215	1217	rBV3	473	399	0.02%	0.002%
20	4.810	1217	1219	1224	rVB4	527	435	0.02%	0.003%
21	4.864	1233	1236	1239	rVB2	389	226	0.01%	0.001%
22	4.948	1259	1262	1264	rBV2	585	372	0.02%	0.002%
23	5.102	1288	1310	1334	rBV2	897044	2138801	100.00%	12.294%
24	5.286	1361	1367	1371	rBV5	536	733	0.03%	0.004%
25	5.350	1385	1387	1390	rBV3	508	378	0.02%	0.002%
26	5.405	1402	1404	1407	rVB2	509	232	0.01%	0.001%
27	5.430	1407	1412	1413	rBV	459	329	0.02%	0.002%
28	5.453	1413	1419	1421	rBV5	889	1075	0.05%	0.006%
29	5.520	1437	1440	1442	rBV	410	229	0.01%	0.001%
30	5.598	1461	1464	1470	rBV3	352	409	0.02%	0.002%
31	5.672	1470	1487	1521	rBV	708907	1413372	66.08%	8.124%
32	5.868	1545	1548	1552	rBV5	833	791	0.04%	0.005%
33	5.951	1562	1574	1586	rVB2	10959	21495	1.01%	0.124%
34	6.009	1589	1592	1594	rBV3	580	348	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007328.D
 Acq On : 01 Sep 2018 02:54
 Operator : SY/MD
 Sample : J4695-14 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.125	1613	1628	1660	rBV	494560	998990	46.71%	5.742%
36	6.434	1719	1724	1727	rBV4	487	455	0.02%	0.003%
37	6.491	1738	1742	1744	rBV2	289	235	0.01%	0.001%
38	6.549	1757	1760	1764	rVB3	470	398	0.02%	0.002%
39	6.581	1767	1770	1771	rBV	330	229	0.01%	0.001%
40	6.607	1775	1778	1780	rBV2	505	325	0.02%	0.002%
41	6.649	1788	1791	1794	rBV2	713	475	0.02%	0.003%
42	6.665	1794	1796	1802	rVB5	719	737	0.03%	0.004%
43	6.739	1812	1819	1820	rBV4	2184	2396	0.11%	0.014%
44	6.974	1889	1892	1894	rBV	430	269	0.01%	0.002%
45	7.035	1894	1911	1938	rVV	231148	414632	19.39%	2.383%
46	7.366	1999	2014	2036	rBV	897750	1585463	74.13%	9.113%
47	7.594	2083	2085	2088	rVB4	636	369	0.02%	0.002%
48	7.668	2096	2108	2130	rBV	162498	286504	13.40%	1.647%
49	7.774	2137	2141	2144	rBV4	670	647	0.03%	0.004%
50	8.147	2245	2257	2292	rBV2	501900	961743	44.97%	5.528%
51	8.514	2367	2371	2377	rVB4	701	616	0.03%	0.004%
52	8.623	2400	2405	2409	rBV2	573	621	0.03%	0.004%
53	8.697	2426	2428	2431	rVB	571	260	0.01%	0.001%
54	8.765	2446	2449	2453	rBV2	351	405	0.02%	0.002%
55	8.816	2461	2465	2467	rBV3	301	265	0.01%	0.002%
56	8.835	2467	2471	2474	rVB3	546	372	0.02%	0.002%
57	8.900	2477	2491	2513	rBV	1032168	1676731	78.40%	9.638%
58	9.150	2567	2569	2572	rVB2	530	276	0.01%	0.002%
59	9.179	2575	2578	2579	rBV3	566	301	0.01%	0.002%
60	9.221	2588	2591	2595	rVB	515	379	0.02%	0.002%
61	9.343	2626	2629	2634	rVB2	367	278	0.01%	0.002%
62	9.427	2650	2655	2659	rBV3	482	533	0.02%	0.003%
63	9.450	2659	2662	2665	rVB2	511	307	0.01%	0.002%
64	9.475	2665	2670	2671	rBV2	351	264	0.01%	0.002%
65	9.504	2676	2679	2686	rVB3	445	432	0.02%	0.002%
66	9.659	2723	2727	2730	rBV2	706	404	0.02%	0.002%
67	9.678	2731	2733	2739	rVV3	371	307	0.01%	0.002%
68	9.739	2747	2752	2755	rVB2	380	412	0.02%	0.002%
69	9.768	2755	2761	2764	rBV3	229	294	0.01%	0.002%
70	9.806	2770	2773	2779	rVB2	273	235	0.01%	0.001%
71	9.839	2779	2783	2784	rBV2	309	224	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007328.D
 Acq On : 01 Sep 2018 02:54
 Operator : SY/MD
 Sample : J4695-14 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	9.913	2804	2806	2811	rBV3	308	258	0.01%	0.001%
73	10.003	2832	2834	2839	rVB3	554	474	0.02%	0.003%
74	10.051	2839	2849	2851	rBV3	546	759	0.04%	0.004%
75	10.179	2885	2889	2893	rVB2	620	430	0.02%	0.002%
76	10.266	2903	2916	2941	rBV	651492	1027915	48.06%	5.908%
77	10.430	2961	2967	2971	rVV2	1198	1406	0.07%	0.008%
78	10.498	2985	2988	2993	rBV2	357	345	0.02%	0.002%
79	10.572	3009	3011	3016	rVB3	442	335	0.02%	0.002%
80	10.697	3047	3050	3054	rBV3	354	295	0.01%	0.002%
81	10.980	3133	3138	3144	rBV4	707	728	0.03%	0.004%
82	11.157	3190	3193	3195	rBV2	451	292	0.01%	0.002%
83	11.208	3206	3209	3212	rVB2	758	524	0.02%	0.003%
84	11.234	3212	3217	3218	rBV3	601	586	0.03%	0.003%
85	11.302	3224	3238	3262	rBV	766408	1242795	58.11%	7.144%
86	11.556	3313	3317	3319	rBV2	582	382	0.02%	0.002%
87	11.572	3320	3322	3326	rVB2	519	260	0.01%	0.001%
88	11.594	3326	3329	3331	rBV2	420	251	0.01%	0.001%
89	11.678	3342	3355	3379	rBV	780593	1253384	58.60%	7.204%
90	12.031	3462	3465	3468	rBV3	488	316	0.01%	0.002%
91	12.125	3491	3494	3496	rBV2	497	234	0.01%	0.001%
92	12.166	3504	3507	3510	rBV4	507	323	0.02%	0.002%
93	12.221	3521	3524	3528	rBV2	448	303	0.01%	0.002%
94	12.285	3542	3544	3548	rVB2	533	303	0.01%	0.002%
95	12.308	3548	3551	3555	rBV3	435	351	0.02%	0.002%
96	12.443	3591	3593	3599	rVB2	908	546	0.03%	0.003%
97	12.482	3601	3605	3610	rBV3	776	688	0.03%	0.004%
98	12.507	3610	3613	3617	rBV2	685	589	0.03%	0.003%
99	13.835	4023	4026	4030	rBV4	1332	1084	0.05%	0.006%
100	13.887	4040	4042	4045	rBV2	872	476	0.02%	0.003%


Sum of corrected areas: 17397397

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007328.D
Acq On : 01 Sep 2018 02:54
Operator : SY/MD
Sample : J4695-14 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

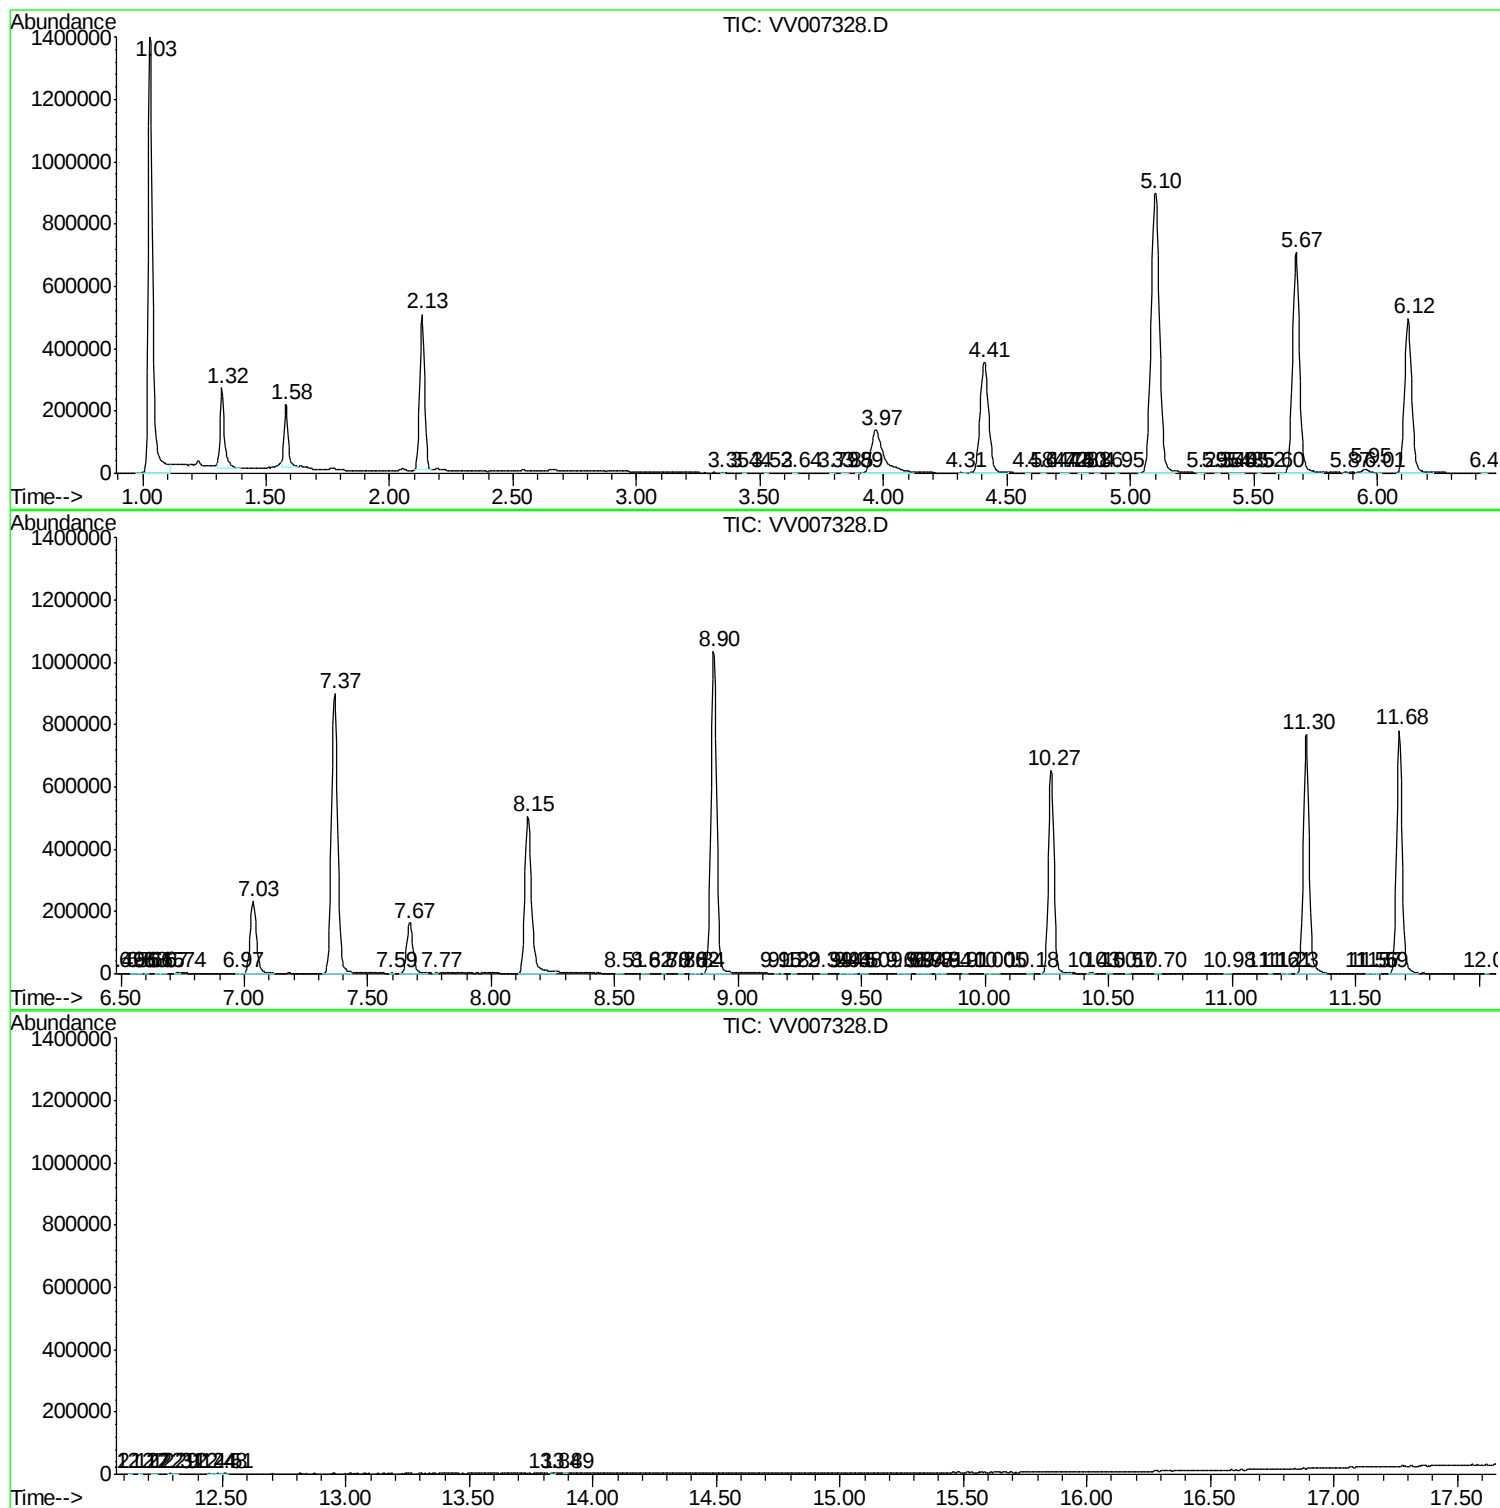

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007328.D
Acq On : 01 Sep 2018 02:54
Operator : SY/MD
Sample : J4695-14 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGA8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007328.D
Acq On : 01 Sep 2018 02:54
Operator : SY/MD
Sample : J4695-14 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
