

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007331.D
 Acq On : 01 Sep 2018 04:07
 Operator : SY/MD
 Sample : J4695-17 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.942	12	16	19	rBV2	390	404	0.002%	0.0002%
2	0.974	23	26	28	rBV2	503	353	0.002%	0.0002%
3	1.032	29	44	66	rBV	1400049	1741414	79.25%	9.799%
4	1.321	127	134	152	rVB	267411	321946	14.65%	1.812%
5	1.578	208	214	232	rVB	209165	241486	10.99%	1.359%
6	2.131	376	386	397	rBV	511928	712207	32.41%	4.008%
7	3.543	822	825	828	rBV	418	285	0.01%	0.0002%
8	3.604	841	844	850	rVB3	694	678	0.03%	0.0004%
9	3.672	860	865	869	rBV3	521	610	0.03%	0.0003%
10	3.913	935	940	941	rBV3	443	373	0.02%	0.0002%
11	3.967	941	957	1011	rVV	138469	515249	23.45%	2.899%
12	4.408	1075	1094	1133	rBV	363723	881898	40.14%	4.962%
13	4.575	1143	1146	1149	rBV2	611	428	0.02%	0.0002%
14	4.620	1157	1160	1162	rBV2	849	497	0.02%	0.0003%
15	4.649	1166	1169	1172	rVB2	866	537	0.02%	0.0003%
16	4.755	1194	1202	1205	rBV3	782	920	0.04%	0.0005%
17	4.874	1237	1239	1243	rBV2	282	268	0.01%	0.0002%
18	4.958	1257	1265	1272	rBV4	660	1110	0.05%	0.0006%
19	5.102	1290	1310	1337	rBV2	922721	2197257	100.00%	12.364%
20	5.311	1373	1375	1378	rBV3	549	291	0.01%	0.0002%
21	5.334	1380	1382	1385	rVB	662	317	0.01%	0.0002%
22	5.408	1403	1405	1408	rVB3	593	352	0.02%	0.0002%
23	5.453	1410	1419	1426	rVB5	1200	1933	0.09%	0.0011%
24	5.507	1426	1436	1437	rBV3	588	542	0.02%	0.0003%
25	5.598	1459	1464	1466	rBV	319	284	0.01%	0.0002%
26	5.671	1470	1487	1514	rBV	715163	1428841	65.03%	8.040%
27	5.951	1563	1574	1584	rBV3	10128	20595	0.94%	0.116%
28	6.006	1588	1591	1594	rBV3	439	286	0.01%	0.0002%
29	6.125	1612	1628	1655	rBV	507380	1025451	46.67%	5.770%
30	6.308	1682	1685	1688	rBV3	626	477	0.02%	0.0003%
31	6.376	1702	1706	1709	rBV3	695	611	0.03%	0.0003%
32	6.549	1754	1760	1766	rBV4	922	1170	0.05%	0.0007%
33	6.578	1766	1769	1772	rBV	397	312	0.01%	0.0002%
34	6.639	1785	1788	1789	rBV2	781	505	0.02%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007331.D
 Acq On : 01 Sep 2018 04:07
 Operator : SY/MD
 Sample : J4695-17 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

35	6.742	1808	1820	1828	rBV4	2425	6052	0.28%	0.034%
36	6.816	1840	1843	1848	rBV4	345	285	0.01%	0.002%
37	6.887	1860	1865	1867	rBV2	483	438	0.02%	0.002%
38	6.906	1869	1871	1874	rVB3	744	400	0.02%	0.002%
39	6.932	1874	1879	1880	rBV	555	409	0.02%	0.002%
40	6.954	1884	1886	1889	rVB2	426	255	0.01%	0.001%
41	6.983	1889	1895	1898	rBV3	622	606	0.03%	0.003%
42	7.035	1898	1911	1932	rBV	232443	421260	19.17%	2.370%
43	7.167	1950	1952	1956	rVB2	773	459	0.02%	0.003%
44	7.221	1968	1969	1974	rBV4	511	304	0.01%	0.002%
45	7.273	1982	1985	1990	rVB3	649	607	0.03%	0.003%
46	7.302	1990	1994	1995	rBV2	381	293	0.01%	0.002%
47	7.366	1999	2014	2046	rBV	941335	1640067	74.64%	9.229%
48	7.562	2072	2075	2079	rBV3	784	468	0.02%	0.003%
49	7.585	2079	2082	2086	rVB4	1043	876	0.04%	0.005%
50	7.617	2086	2092	2093	rBV4	585	421	0.02%	0.002%
51	7.668	2093	2108	2137	rBV	169200	293972	13.38%	1.654%
52	7.810	2150	2152	2154	rBV3	669	347	0.02%	0.002%
53	7.861	2166	2168	2170	rBV3	541	314	0.01%	0.002%
54	8.147	2244	2257	2284	rBV2	527150	976598	44.45%	5.495%
55	8.414	2338	2340	2350	rVB8	1560	1642	0.07%	0.009%
56	8.507	2367	2369	2371	rVB2	632	281	0.01%	0.002%
57	8.520	2371	2373	2375	rBV2	528	290	0.01%	0.002%
58	8.658	2411	2416	2419	rVB3	576	542	0.02%	0.003%
59	8.752	2442	2445	2451	rVB4	784	731	0.03%	0.004%
60	8.810	2461	2463	2469	rVB3	460	386	0.02%	0.002%
61	8.900	2477	2491	2513	rBV	1032484	1693530	77.07%	9.529%
62	9.170	2572	2575	2576	rVV2	577	290	0.01%	0.002%
63	9.183	2577	2579	2582	rVB2	756	450	0.02%	0.003%
64	9.218	2587	2590	2592	rBV4	687	430	0.02%	0.002%
65	9.234	2592	2595	2599	rVB2	730	415	0.02%	0.002%
66	9.327	2620	2624	2627	rVB3	483	303	0.01%	0.002%
67	9.385	2640	2642	2647	rVB3	533	421	0.02%	0.002%
68	9.437	2654	2658	2662	rBV2	557	438	0.02%	0.002%
69	9.617	2709	2714	2718	rBV2	489	569	0.03%	0.003%
70	9.639	2718	2721	2723	rVV2	533	347	0.02%	0.002%
71	9.928	2807	2811	2814	rVB3	389	300	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007331.D
 Acq On : 01 Sep 2018 04:07
 Operator : SY/MD
 Sample : J4695-17 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis

72	10.006	2831	2835	2839	rBV2	397	403	0.02%	0.002%
73	10.266	2904	2916	2935	rBV	662443	1044432	47.53%	5.877%
74	10.427	2959	2966	2969	rBV4	1430	1443	0.07%	0.008%
75	10.572	3008	3011	3013	rBV2	439	263	0.01%	0.001%
76	10.687	3044	3047	3050	rBV	420	312	0.01%	0.002%
77	10.764	3067	3071	3076	rVB3	612	604	0.03%	0.003%
78	10.790	3076	3079	3083	rBV	381	382	0.02%	0.002%
79	10.813	3083	3086	3090	rBV2	435	369	0.02%	0.002%
80	10.903	3112	3114	3116	rBV	621	318	0.01%	0.002%
81	11.019	3147	3150	3156	rBV3	465	461	0.02%	0.003%
82	11.102	3171	3176	3181	rVB4	428	509	0.02%	0.003%
83	11.125	3181	3183	3187	rVB2	416	272	0.01%	0.002%
84	11.166	3194	3196	3202	rBV3	386	321	0.01%	0.002%
85	11.250	3216	3222	3225	rBV3	362	430	0.02%	0.002%
86	11.301	3225	3238	3261	rBV	784522	1262031	57.44%	7.101%
87	11.456	3282	3286	3288	rBV3	485	402	0.02%	0.002%
88	11.678	3342	3355	3378	rBV	802945	1292574	58.83%	7.273%
89	11.980	3446	3449	3453	rBV2	746	588	0.03%	0.003%
90	12.131	3494	3496	3500	rVB3	573	288	0.01%	0.002%
91	12.227	3521	3526	3530	rBV2	862	802	0.04%	0.005%
92	12.250	3530	3533	3536	rBV3	495	429	0.02%	0.002%
93	12.330	3554	3558	3560	rBV2	461	374	0.02%	0.002%
94	12.375	3570	3572	3578	rVB3	536	512	0.02%	0.003%
95	12.906	3733	3737	3738	rBV3	385	297	0.01%	0.002%
96	12.986	3758	3762	3766	rBV	27318	14664	0.67%	0.083%
97	13.038	3775	3778	3782	rBV3	718	588	0.03%	0.003%
98	13.179	3819	3822	3824	rBV2	512	294	0.01%	0.002%
99	13.285	3853	3855	3858	rBV	453	345	0.02%	0.002%
100	14.002	4075	4078	4085	rVB6	1016	1253	0.06%	0.007%


Sum of corrected areas: 17771643

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083118\
Data File : VV007331.D
Acq On : 01 Sep 2018 04:07
Operator : SY/MD
Sample : J4695-17 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

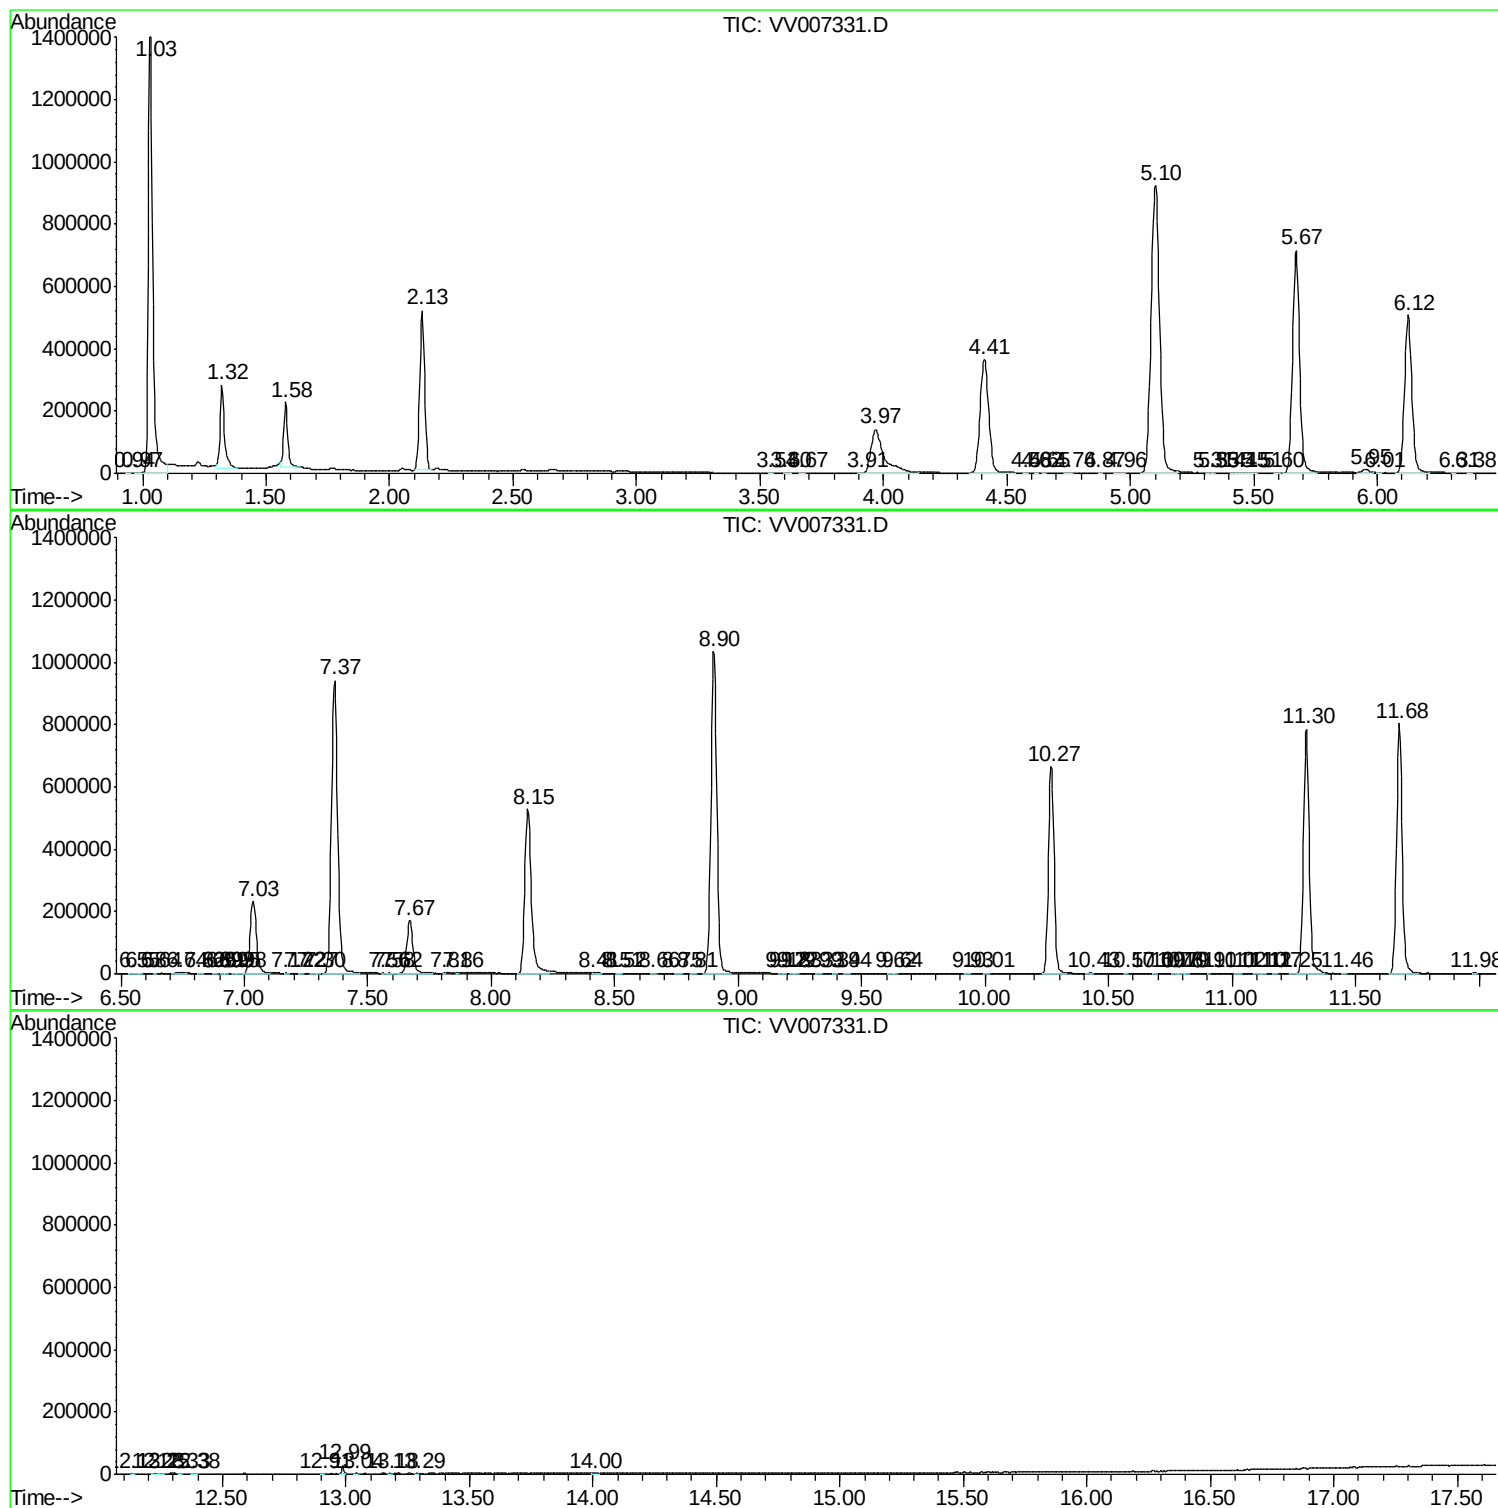

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083118\
Data File : VV007331.D
Acq On : 01 Sep 2018 04:07
Operator : SY/MD
Sample : J4695-17 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV083118\
Data File : VV007331.D
Acq On : 01 Sep 2018 04:07
Operator : SY/MD
Sample : J4695-17 50X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEGB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM083118WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc