


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083118\
 Data File : VV007288.D
 Acq On : 31 Aug 2018 08:53
 Operator : SY/MD
 Sample : BFB70
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM083118WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 01 01:00:35 2018

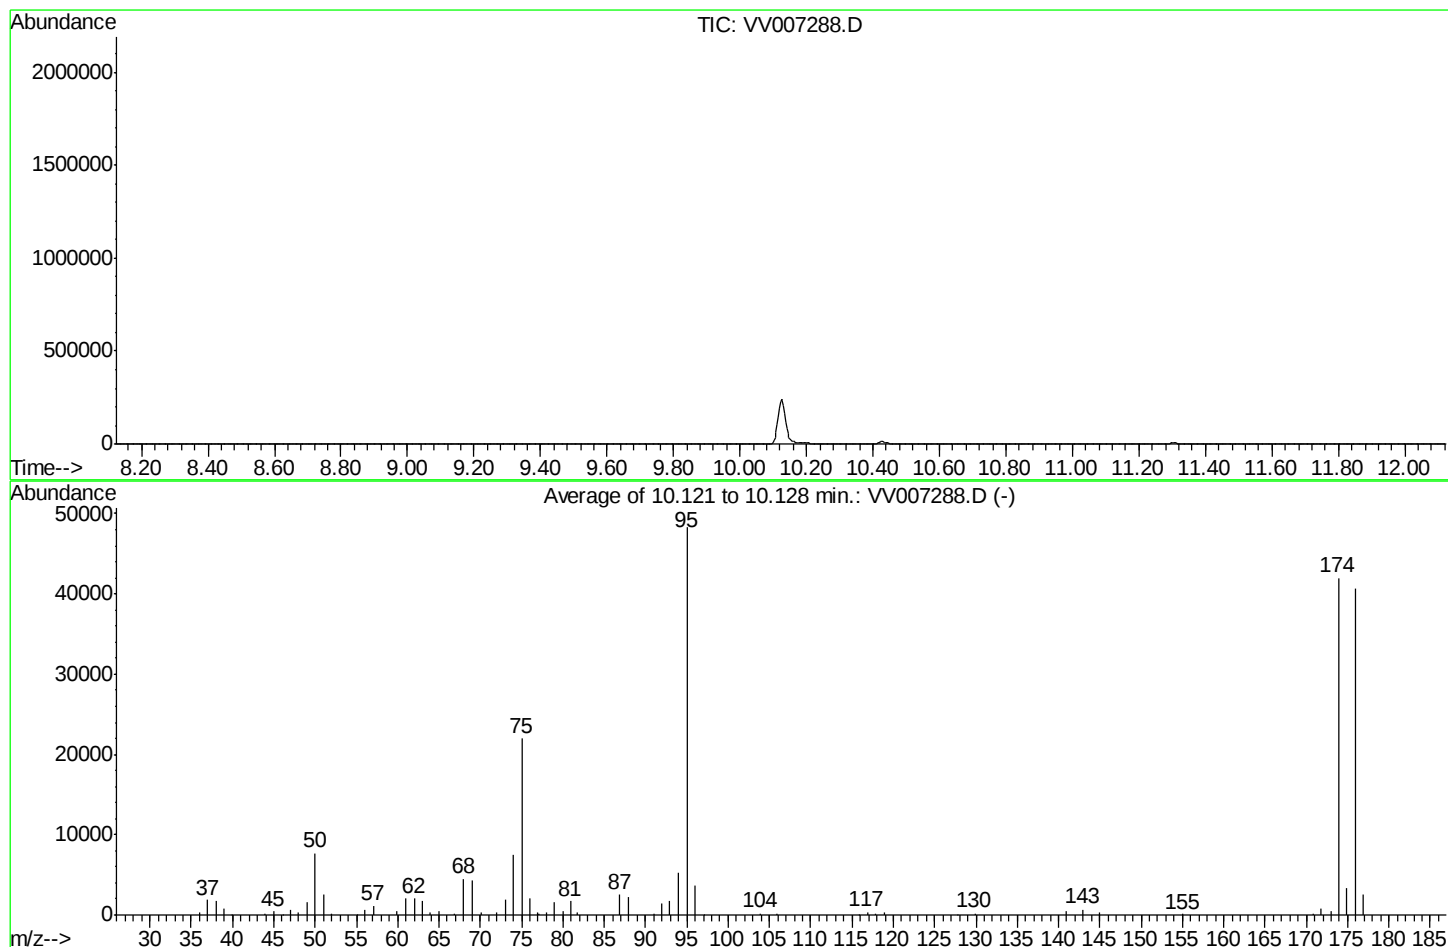

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	7708	PASS
75	95	30	80	45.4	21949	PASS
95	95	100	100	100.0	48296	PASS
96	95	5	9	7.5	3610	PASS
173	174	0.00	2	1.2	501	PASS
174	95	50	120	87.0	42024	PASS
175	174	5	9	8.1	3411	PASS
176	174	95	101	96.6	40616	PASS
177	176	5	9	6.1	2479	PASS

Scan 2860 (10.086 min): VV007288.D
BFB70

m/z	Abundance
39.90	349.0
43.90	648.0
207.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	282.0
37.00	2012.0
38.00	1648.0
39.00	874.0
40.00	39 .0
43.90	893.0
4 .00	433.0
46.10	12 .0
46.90	678.0
47.90	263.0
49.00	1687.0
0.00	7841.0
1.00	2 4 .0
6.00	8 .0
7.10	106 .0
9.90	46.0
61.00	1967.0
62.00	20 2.0
63.00	1819.0
63.90	33 .0
6 .10	439.0
66.90	169.0
68.00	4301.0
69.00	424 .0
70.00	394.0
71.90	276.0
73.00	1763.0
74.00	7171.0
7 .00	21640.0
76.00	2111.0
76.90	342.0
78.00	331.0
78.90	1626.0
80.00	397.0
80.90	1731.0
81.80	33 .0
86.90	2320.0
88.00	2097.0
91.00	234.0
91.90	1341.0
92.90	1627.0
94.00	181.0
9 .00	47144.0
96.00	3661.0
104.00	172.0
10 .90	141.0
116.90	370.0
117.80	177.0
118.90	28 .0
127.70	116.0
129.80	1 .0
140.90	496.0
143.00	49.0
144.90	397.0
1 .10	139.0
170.80	144.0
171.80	7 6.0
173.00	48 .0
173.90	40328.0
174.90	3109.0
17 .90	38896.0
176.90	2340.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
3 .90	292.0
37.00	1900.0
38.00	1690.0
39.00	898.0
39.90	380.0
43.90	887.0
4 .00	442.0
47.00	703.0
47.90	298.0
49.00	16 .9.0
0.00	7963.0
1.00	26 .9.0
2.00	112.0
.10	107.0
6.00	61 .0
7.00	1203.0
9.90	87.0
61.00	2113.0
62.00	2108.0
63.00	1903.0
64.00	318.0
6 .10	483.0
66.80	1 .8.0
68.00	4696.0
69.00	4466.0
70.10	389.0
71.90	29 .0
73.00	204 .0
74.00	77 7.0
7 .00	22664.0
76.00	2214.0
76.90	306.0
78.00	383.0
78.90	1681.0
80.00	406.0
80.90	1781.0
81.80	370.0
86.90	2 .4.0
88.00	2303.0
91.00	213.0
91.90	1429.0
93.00	17 3.0
94.00	314.0
9 .00	0112.0
96.00	3782.0
97.00	102.0
103.90	184.0
106.00	162.0
116.80	327.0
117.80	19 .0
118.90	308.0
127.80	109.0
129.80	164.0
141.00	19.0
143.00	7 .9.0
144.90	402.0
1 .10	129.0
170.80	126.0
171.80	820.0
173.00	20.0
173.90	43360.0
174.90	3 34.0
17 .90	41800.0
177.00	2 64.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	317.0
37.00	1666.0
38.00	1723.0
39.00	787.0
39.90	382.0
43.90	844.0
4 .00	381.0
46.00	121.0
46.90	83.0
47.90	270.0
49.00	1 29.0
0.00	7321.0
1.00	2481.0
2.00	149.0
.10	107.0
6.00	7.0
7.00	1206.0
9.90	487.0
61.00	1980.0
62.00	19 2.0
63.00	1771.0
64.00	287.0
6 .00	27.0
66.90	1 8.0
68.00	4419.0
69.00	4299.0
70.10	3 0.0
71.90	297.0
73.00	2074.0
74.00	7462.0
7 .00	21 44.0
76.00	2136.0
76.90	28 .0
77.10	291.0
78.00	349.0
78.90	1623.0
79.90	44 .0
80.90	1649.0
81.80	380.0
86.90	2 82.0
87.90	22 0.0
91.00	199.0
91.90	1318.0
93.00	1841.0
94.00	07 .0
9 .00	47632.0
96.00	3388.0
103.90	173.0
106.00	172.0
11 .80	118.0
116.80	276.0
117.90	182.0
118.80	309.0
129.90	16 .0
141.00	4 .0
143.00	82 .0
144.90	3 2.0
170.90	109.0
171.80	791.0
173.00	00.0
173.90	42384.0
174.90	3 91.0
17 .90	411 2.0
177.00	2 3 .0
206.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70