

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083121\
 Data File : VW022034.D
 Acq On : 31 Aug 2021 12:06
 Operator : SY/MD
 Sample : M3579-06MEDL 100X
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8MEDL

Quant Time: Sep 01 02:43:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 01 02:41:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	348056	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	334992	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	168273	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	84941	35.240	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.480%		
7) Chloroethane-d5	1.561	69	79224	42.089	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.180%		
11) 1,1-Dichloroethene-d2	2.105	63	123894	31.080	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.160%		
21) 2-Butanone-d5	3.876	46	167801	101.510	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.510%		
24) Chloroform-d	4.349	84	184599	42.002	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.000%		
26) 1,2-Dichloroethane-d4	5.034	65	122832	47.449	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.900%		
32) Benzene-d6	5.050	84	410671	45.198	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.400%		
36) 1,2-Dichloropropane-d6	6.072	67	133400	46.685	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.360%		
41) Toluene-d8	7.320	98	377839	44.052	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.100%		
43) trans-1,3-Dichloroprop...	7.625	79	56594	41.612	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.220%		
47) 2-Hexanone-d5	8.088	63	100117	91.314	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.310%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	174664	47.727	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.460%		
66) 1,2-Dichlorobenzene-d4	11.628	152	158626	47.951	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.900%		
Target Compounds					Qvalue	
25) Chloroform	4.381	83	17310	3.782	ug/L	95
46) Tetrachloroethene	7.982	164	4768	2.221	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
Data File : VV022034.D
Acq On : 31 Aug 2021 12:06
Operator : SY/MD
Sample : M3579-06MEDL 100X
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8MEDL

Quant Time: Sep 01 02:43:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 01 02:41:24 2021
Response via : Initial Calibration

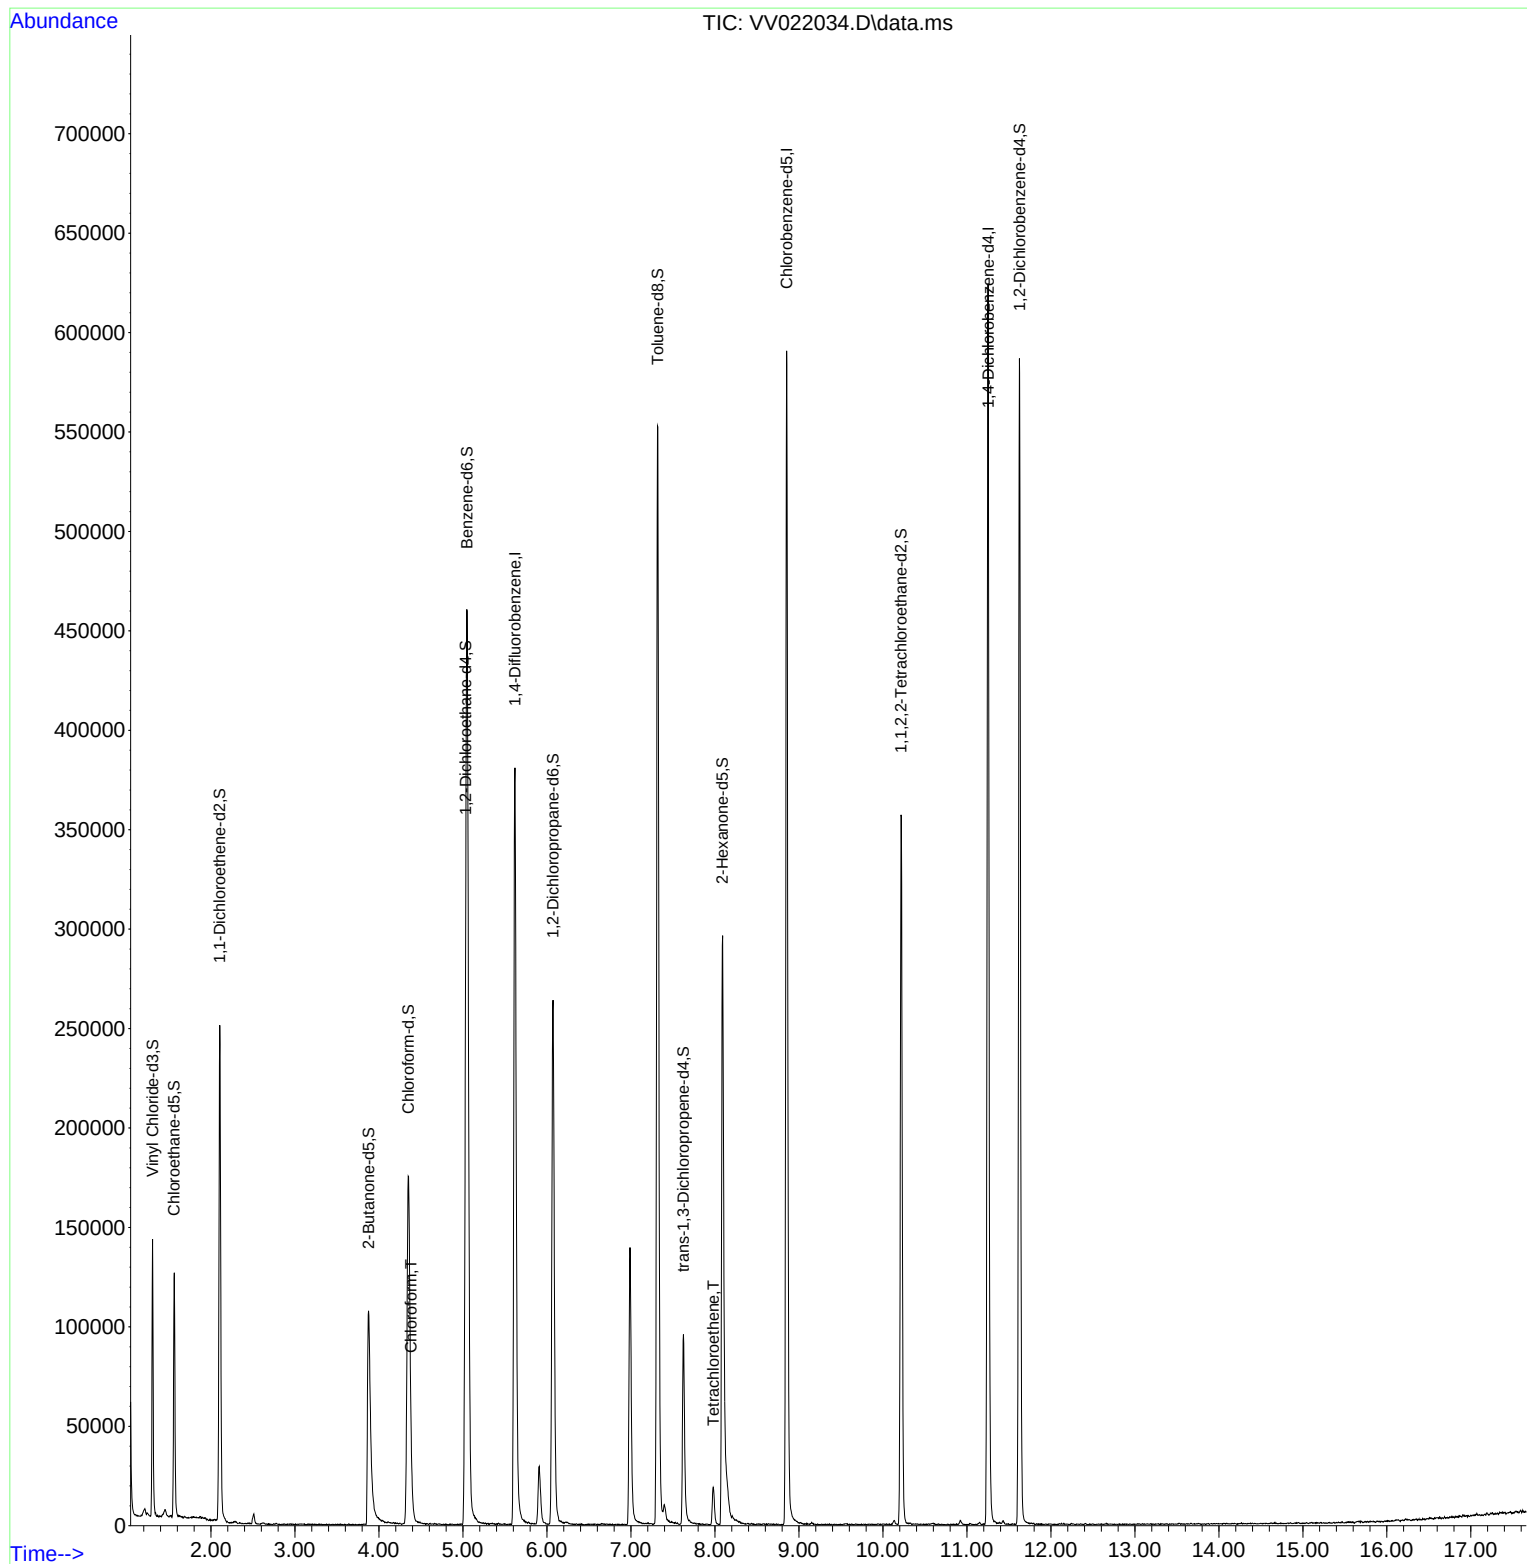




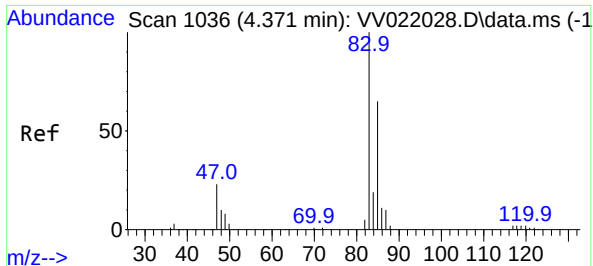


#25

Chloroform
Concen: 3.782 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.010 min
Lab File: VV022034.D
Acq: 31 Aug 2021 12:06

Instrument :
MSVOA_V
ClientSampleId :
GB6A8MEDL

Tgt Ion: 83 Resp: 17310
Ion Ratio Lower Upper
83 100
85 62.4 46.3 85.9

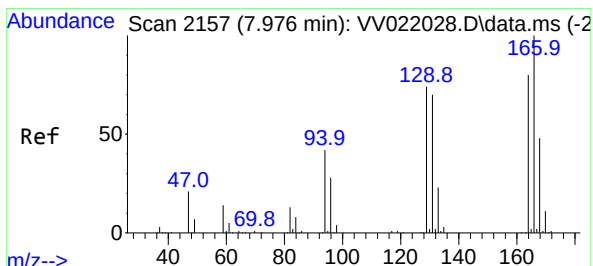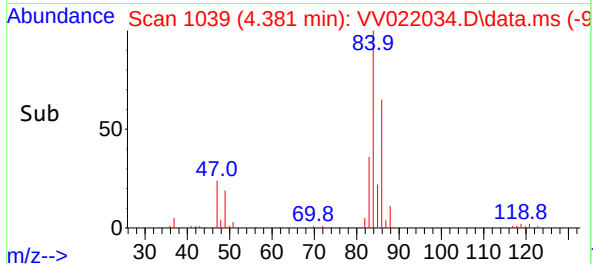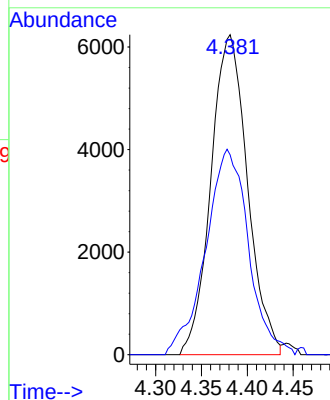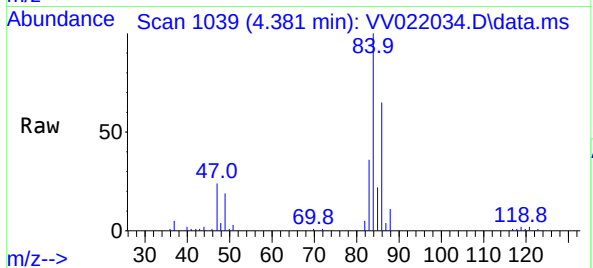

#46

Tetrachloroethene
Concen: 2.221 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. 0.007 min
Lab File: VV022034.D
Acq: 31 Aug 2021 12:06

Tgt Ion:164 Resp: 4768
Ion Ratio Lower Upper
164 100
129 95.3 62.9 116.9
131 91.4 61.0 113.4
166 121.7 90.6 168.3

