

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
 Data File : VV022053.D
 Acq On : 31 Aug 2021 20:10
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	106	rVB	72994	99349	3.00%	0.833%
2	2.076	313	322	334	rVB	165349	236787	7.14%	1.985%
3	2.616	480	490	503	rVB	13736	27738	0.84%	0.233%
4	2.815	547	552	553	rBV3	699	475	0.01%	0.004%
5	3.040	621	622	626	rBV3	511	296	0.01%	0.002%
6	3.085	633	636	641	rBV2	383	268	0.01%	0.002%
7	3.121	644	647	649	rVB	381	213	0.01%	0.002%
8	3.137	649	652	657	rBV2	675	552	0.02%	0.005%
9	3.397	728	733	736	rBV4	601	599	0.02%	0.005%
10	3.442	745	747	752	rBV2	291	181	0.01%	0.002%
11	3.491	760	762	766	rVB2	358	215	0.01%	0.002%
12	3.565	779	785	786	rBV2	279	220	0.01%	0.002%
13	3.716	828	832	835	rBV3	487	335	0.01%	0.003%
14	3.780	850	852	855	rBV2	267	183	0.01%	0.002%
15	3.793	855	856	859	rBV	381	212	0.01%	0.002%
16	3.889	875	886	916	rBV	71906	258336	7.79%	2.166%
17	4.346	1012	1028	1061	rBV	146192	387481	11.69%	3.248%
18	4.581	1097	1101	1102	rBV2	455	353	0.01%	0.003%
19	4.587	1102	1103	1106	rVB2	846	312	0.01%	0.003%
20	4.661	1121	1126	1128	rBV5	779	564	0.02%	0.005%
21	4.754	1146	1155	1158	rBV4	402	544	0.02%	0.005%
22	4.806	1167	1171	1172	rBV	327	206	0.01%	0.002%
23	4.828	1177	1178	1182	rBV	360	233	0.01%	0.002%
24	5.040	1228	1244	1280	rVV2	381334	957638	28.88%	8.028%
25	5.236	1303	1305	1309	rBV3	510	358	0.01%	0.003%
26	5.307	1323	1327	1330	rBV2	507	402	0.01%	0.003%
27	5.339	1332	1337	1339	rBV5	1145	924	0.03%	0.008%
28	5.523	1391	1394	1396	rBV2	282	225	0.01%	0.002%
29	5.613	1407	1422	1452	rBV	386721	810452	24.44%	6.794%
30	5.908	1502	1514	1535	rBV5	31171	77308	2.33%	0.648%
31	6.069	1551	1564	1599	rVB	214140	456280	13.76%	3.825%
32	6.310	1635	1639	1640	rBV2	530	301	0.01%	0.003%
33	6.365	1653	1656	1658	rBV2	519	335	0.01%	0.003%
34	6.417	1670	1672	1677	rBV	521	348	0.01%	0.003%
35	6.452	1681	1683	1685	rBV2	576	271	0.01%	0.002%
36	6.487	1690	1694	1696	rBV2	359	242	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083121\
 Data File : VW022053.D
 Acq On : 31 Aug 2021 20:10
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.500	1696	1698	1701	rBV	324	234	0.01%	0.002%
38	6.751	1773	1776	1779	rBV3	654	376	0.01%	0.003%
39	6.809	1790	1794	1797	rBV3	480	364	0.01%	0.003%
40	6.841	1803	1804	1808	rVB	547	245	0.01%	0.002%
41	6.989	1838	1850	1879	rBV	104163	210009	6.33%	1.760%
42	7.201	1912	1916	1917	rBV2	724	488	0.01%	0.004%
43	7.256	1926	1933	1935	rBV7	1268	1242	0.04%	0.010%
44	7.269	1935	1937	1940	rVB2	570	346	0.01%	0.003%
45	7.317	1940	1952	1973	rBV	410758	733749	22.13%	6.151%
46	7.625	2038	2048	2071	rBV	68637	136653	4.12%	1.146%
47	7.863	2118	2122	2125	rBV2	457	347	0.01%	0.003%
48	7.976	2143	2157	2183	rBV	1957752	3315440	100.00%	27.792%
49	8.105	2186	2197	2238	rVB2	260585	614907	18.55%	5.155%
50	8.481	2311	2314	2317	rBV3	415	273	0.01%	0.002%
51	8.506	2320	2322	2324	rBV2	354	210	0.01%	0.002%
52	8.571	2340	2342	2345	rVV3	483	338	0.01%	0.003%
53	8.587	2345	2347	2350	rVB	486	225	0.01%	0.002%
54	8.687	2375	2378	2381	rVB3	351	282	0.01%	0.002%
55	8.706	2381	2384	2387	rBV2	277	205	0.01%	0.002%
56	8.767	2399	2403	2406	rVB2	569	474	0.01%	0.004%
57	8.789	2406	2410	2412	rBV	444	243	0.01%	0.002%
58	8.854	2418	2430	2453	rBV	580984	1017987	30.70%	8.533%
59	9.156	2520	2524	2531	rVB5	1520	1715	0.05%	0.014%
60	9.233	2544	2548	2551	rBV2	391	234	0.01%	0.002%
61	9.378	2590	2593	2598	rBV3	288	225	0.01%	0.002%
62	9.461	2616	2619	2624	rBV4	393	337	0.01%	0.003%
63	9.529	2637	2640	2644	rBV2	305	256	0.01%	0.002%
64	9.555	2644	2648	2649	rVV3	363	251	0.01%	0.002%
65	9.600	2660	2662	2665	rBV	399	235	0.01%	0.002%
66	9.683	2682	2688	2691	rBV3	199	201	0.01%	0.002%
67	9.706	2692	2695	2699	rVB	425	316	0.01%	0.003%
68	9.731	2699	2703	2705	rBV2	282	254	0.01%	0.002%
69	9.921	2756	2762	2763	rBV3	460	340	0.01%	0.003%
70	9.947	2768	2770	2774	rVV	684	455	0.01%	0.004%
71	9.963	2774	2775	2779	rVB	562	203	0.01%	0.002%
72	9.985	2779	2782	2785	rVB2	253	186	0.01%	0.002%
73	10.088	2809	2814	2817	rBV2	315	238	0.01%	0.002%
74	10.127	2822	2826	2830	rBV3	751	813	0.02%	0.007%
75	10.223	2842	2856	2871	rBV	352347	570256	17.20%	4.780%
76	10.387	2904	2907	2910	rBV2	471	309	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
 Data File : VV022053.D
 Acq On : 31 Aug 2021 20:10
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.545	2949	2956	2961	rBV3	695	1080	0.03%	0.009%
78	10.635	2980	2984	2986	rBV	519	288	0.01%	0.002%
79	10.748	3016	3019	3021	rBV2	295	181	0.01%	0.002%
80	10.883	3057	3061	3066	rBV2	342	361	0.01%	0.003%
81	10.908	3066	3069	3070	rVV	536	350	0.01%	0.003%
82	10.924	3070	3074	3084	rVV6	1867	2555	0.08%	0.021%
83	11.143	3139	3142	3149	rVB3	677	542	0.02%	0.005%
84	11.191	3152	3157	3165	rBV5	1240	1604	0.05%	0.013%
85	11.252	3165	3176	3204	rBV	715189	1118852	33.75%	9.379%
86	11.468	3239	3243	3244	rBV	359	216	0.01%	0.002%
87	11.542	3265	3266	3269	rVV2	410	228	0.01%	0.002%
88	11.629	3281	3293	3314	rBV	550926	865509	26.11%	7.255%
89	11.821	3349	3353	3355	rBV3	593	466	0.01%	0.004%
90	12.233	3479	3481	3482	rBV3	456	199	0.01%	0.002%
91	12.384	3526	3528	3532	rVV2	270	191	0.01%	0.002%
92	12.432	3539	3543	3548	rVB5	379	438	0.01%	0.004%
93	12.481	3555	3558	3560	rBV2	375	253	0.01%	0.002%
94	12.780	3648	3651	3653	rBV	682	433	0.01%	0.004%
95	12.886	3681	3684	3690	rBV4	612	421	0.01%	0.004%
96	13.268	3800	3803	3809	rBV4	806	912	0.03%	0.008%
97	13.336	3821	3824	3826	rBV2	248	180	0.01%	0.002%
98	13.519	3876	3881	3890	rBV4	771	1062	0.03%	0.009%
99	13.599	3901	3906	3908	rBV3	398	341	0.01%	0.003%
100	13.709	3935	3940	3941	rBV2	547	477	0.01%	0.004%

Sum of corrected areas: 11929336




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
Data File : VV022053.D
Acq On : 31 Aug 2021 20:10
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

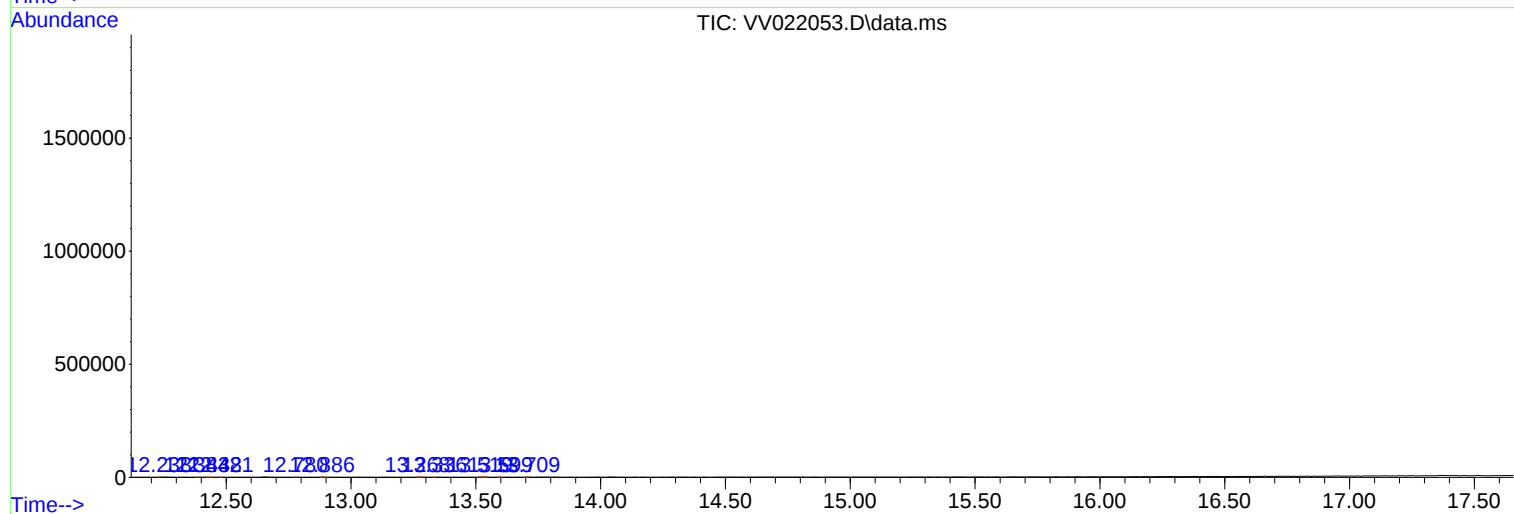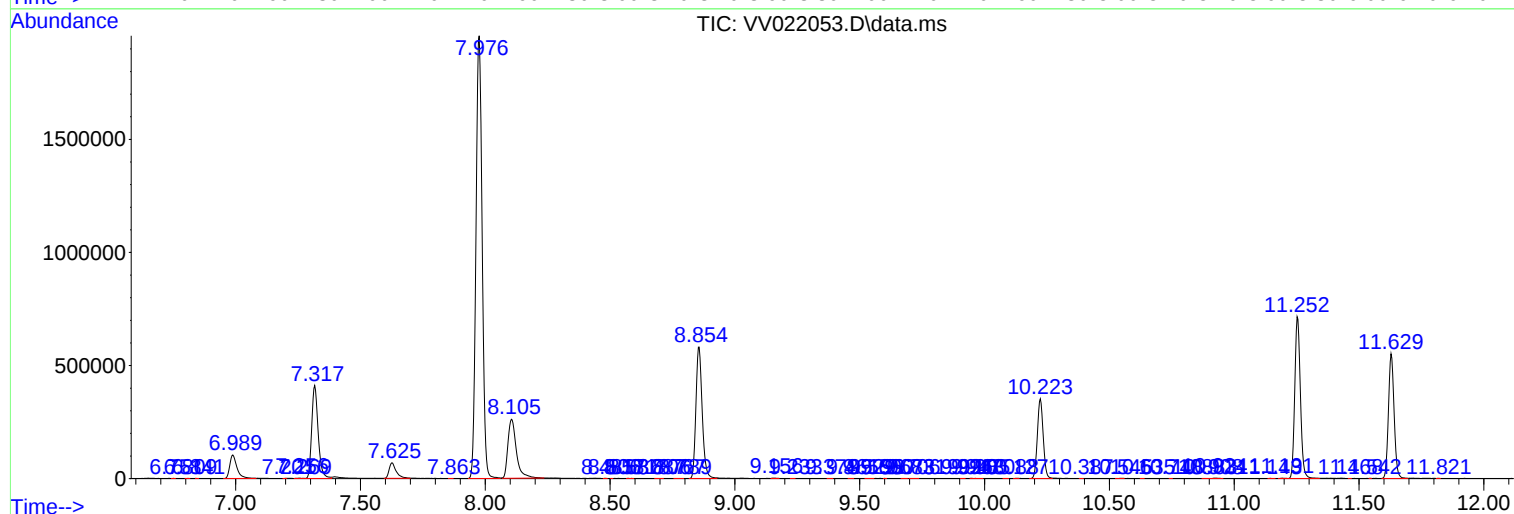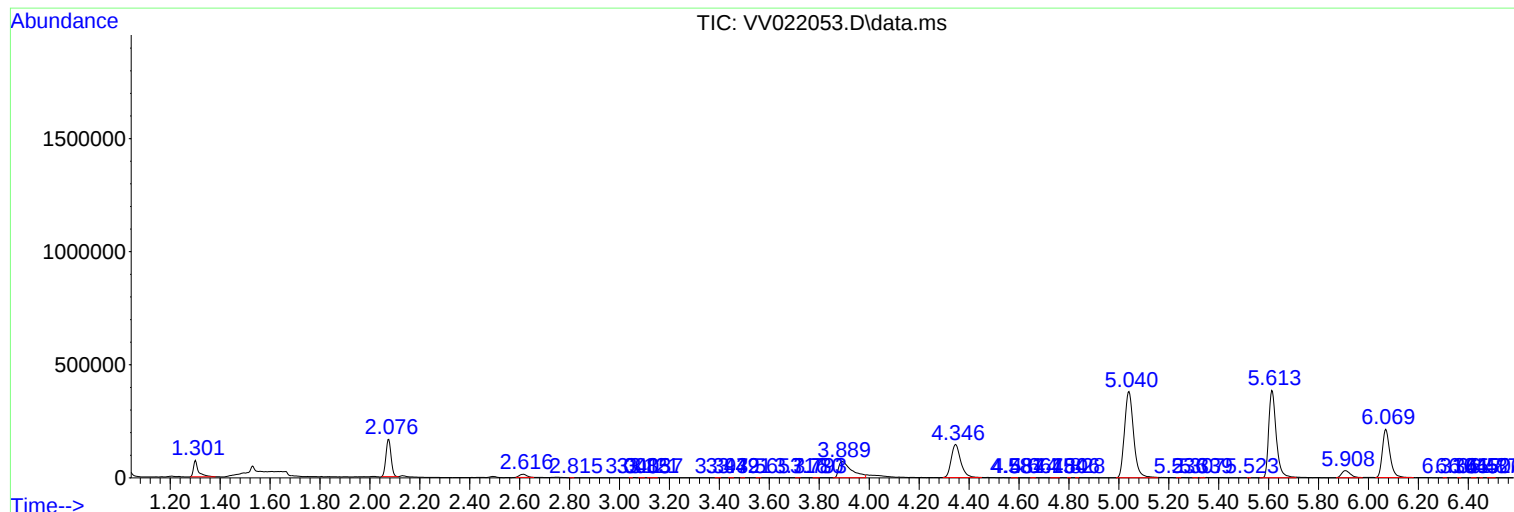

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
Data File : VV022053.D
Acq On : 31 Aug 2021 20:10
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
Data File : VV022053.D
Acq On : 31 Aug 2021 20:10
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
