
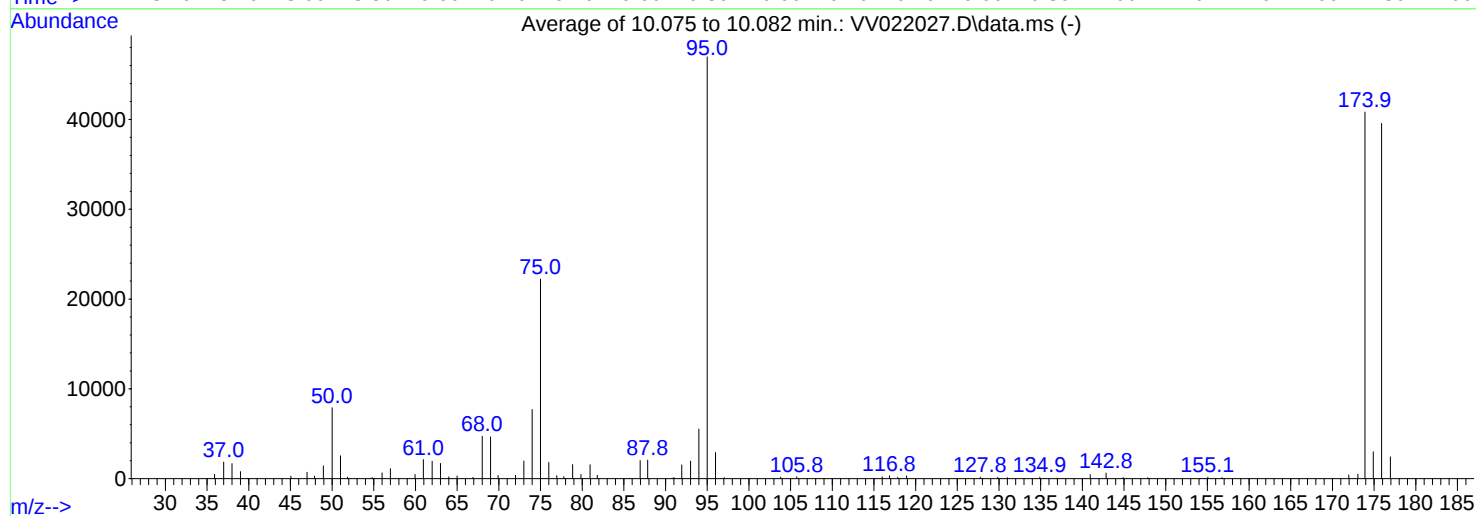


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083121\
Data File : VV022027.D
Acq On : 31 Aug 2021 08:57
Operator : SY/MD
Sample : BFB225
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB225

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis
Last Update : Thu Sep 02 05:24:11 2021

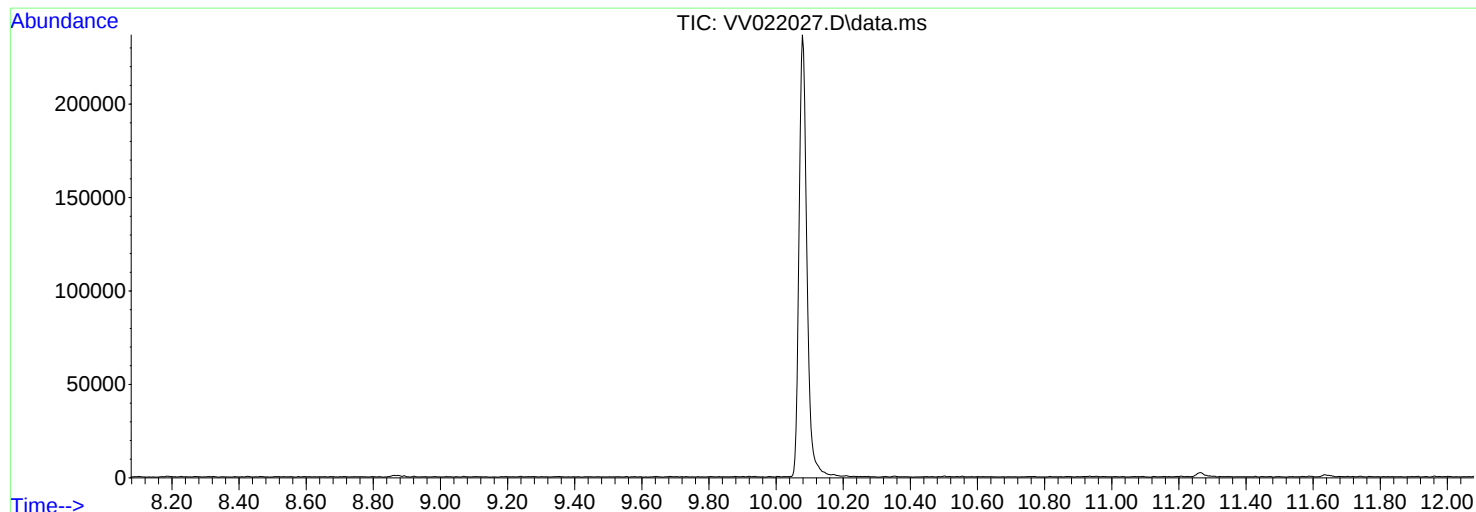

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	7886	PASS
75	95	30	80	47.3	22224	PASS
95	95	100	100	100.0	46973	PASS
96	95	5	9	6.2	2901	PASS
173	174	0.00	2	1.2	500	PASS
174	95	50	120	86.9	40821	PASS
175	174	5	9	7.3	2991	PASS
176	174	95	105	96.9	39565	PASS
177	176	5	10	6.1	2417	PASS

m/z	Abundance
35.90	508.0
37.00	1784.0
38.00	1623.0
39.00	681.0
39.90	234.0
44.00	443.0
45.00	283.0
47.00	652.0
47.90	239.0
49.00	1478.0
50.00	7609.0
51.00	2499.0
51.80	170.0
54.80	138.0
56.00	697.0
57.00	1024.0
60.00	462.0
60.90	1962.0
62.00	1945.0
63.00	1681.0
64.00	194.0
65.00	326.0
66.90	114.0
68.00	4499.0
69.00	4703.0
69.90	311.0
72.00	366.0
73.00	1942.0
74.00	7377.0
75.00	21744.0
76.00	1658.0
77.00	326.0
77.90	248.0
78.90	1491.0
79.90	459.0
80.90	1587.0
81.80	369.0
85.70	102.0
86.90	1890.0
87.90	1963.0
91.00	191.0
92.00	1574.0
93.00	2070.0
94.00	5446.0
95.00	46416.0
96.00	2761.0
97.10	103.0
103.80	146.0
105.80	223.0
115.10	110.0
116.00	224.0
116.80	327.0
117.80	173.0
118.90	309.0
127.80	214.0
129.90	184.0
131.00	103.0
134.90	100.0
136.90	112.0
141.00	386.0
142.80	606.0
144.90	115.0
147.80	118.0
155.00	138.0
156.70	105.0
172.00	463.0
173.00	541.0
173.90	42256.0
174.90	2990.0
175.90	40432.0
177.00	2380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
35.90	480.0
37.00	1918.0
38.00	1727.0
39.00	790.0
39.80	244.0
44.10	462.0
45.10	311.0
47.00	778.0
47.90	270.0
49.00	1426.0
50.00	8117.0
51.00	2656.0
51.80	198.0
54.80	144.0
56.00	663.0
57.00	1159.0
59.90	466.0
61.00	2170.0
62.00	1960.0
63.00	1769.0
64.00	200.0
65.00	320.0
66.90	154.0
68.00	4938.0
69.00	4851.0
69.90	366.0
72.00	392.0
73.00	1997.0
74.00	8020.0
75.00	22944.0
76.00	1844.0
76.90	332.0
77.80	216.0
78.90	1603.0
79.80	481.0
80.90	1611.0
81.80	394.0
86.90	2031.0
87.90	2177.0
91.00	191.0
92.00	1563.0
93.00	2011.0
94.00	5713.0
95.00	48656.0
96.00	2962.0
97.10	106.0
103.80	181.0
105.70	206.0
116.00	194.0
116.90	331.0
117.80	159.0
118.90	311.0
127.80	189.0
129.90	160.0
131.00	121.0
134.90	172.0
140.90	463.0
142.80	645.0
144.90	134.0
147.90	121.0
155.10	175.0
156.80	140.0
171.90	408.0
173.00	506.0
173.90	42072.0
174.90	3105.0
175.90	40880.0
176.90	2506.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
39.90	212.0
44.00	463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
35.90	449.0
37.00	1875.0
38.00	1667.0
39.00	860.0
39.90	261.0
44.00	470.0
45.00	287.0
47.00	737.0
47.90	296.0
48.90	1357.0
50.00	7931.0
51.00	2487.0
51.90	165.0
54.80	109.0
56.00	583.0
57.00	1148.0
59.90	468.0
61.00	2223.0
62.00	1923.0
63.00	1648.0
64.00	173.0
65.00	292.0
66.90	177.0
68.00	4713.0
69.00	4398.0
69.90	372.0
72.00	354.0
73.00	1938.0
74.00	7701.0
75.00	21984.0
76.00	1909.0
76.90	339.0
77.70	228.0
78.80	1609.0
79.80	475.0
81.00	1473.0
81.80	360.0
87.00	2122.0
87.80	2047.0
90.80	152.0
91.90	1456.0
93.00	1816.0
94.00	5404.0
95.00	45848.0
96.00	2979.0
97.00	111.0
103.80	191.0
105.80	205.0
116.00	187.0
116.80	286.0
117.90	142.0
118.90	284.0
127.70	140.0
128.10	129.0
129.80	116.0
131.00	104.0
134.90	196.0
141.00	502.0
142.90	639.0
144.90	119.0
147.90	112.0
154.70	130.0
155.10	174.0
156.80	140.0
172.00	343.0
173.10	453.0
173.90	38136.0
174.90	2878.0
175.90	37384.0
176.90	2366.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225