




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027638.D
Acq On : 01 Sep 2022 00:42
Operator : SY/MD
Sample : N4366-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 01 04:16:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:22:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

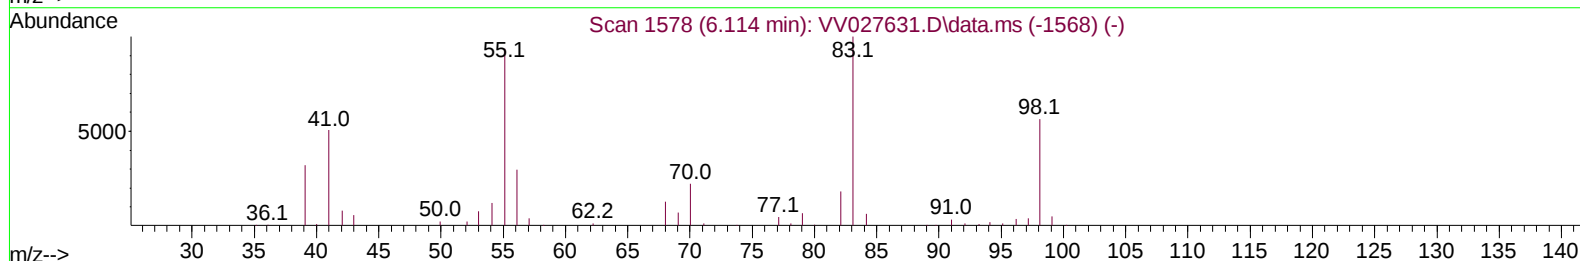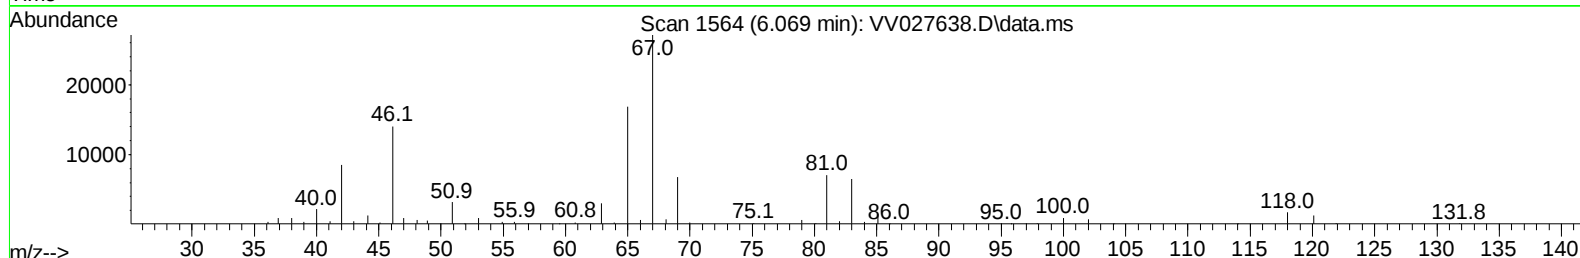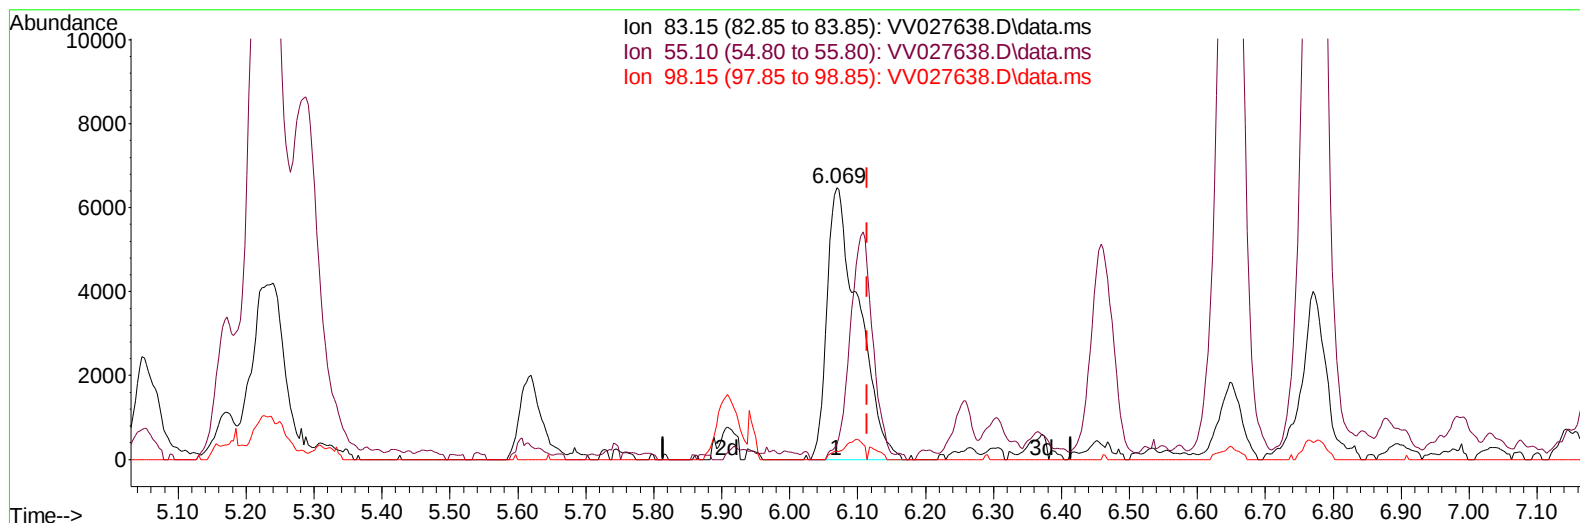

TIC: VV027638.D\data.ms

(35) Methylcyclohexane (T)

6.069min (-0.045) 0.96 ug/L

response 20790

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	0.00#
98.15	46.10	5.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027638.D
 Acq On : 01 Sep 2022 00:42
 Operator : SY/MD
 Sample : N4366-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 01 04:16:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

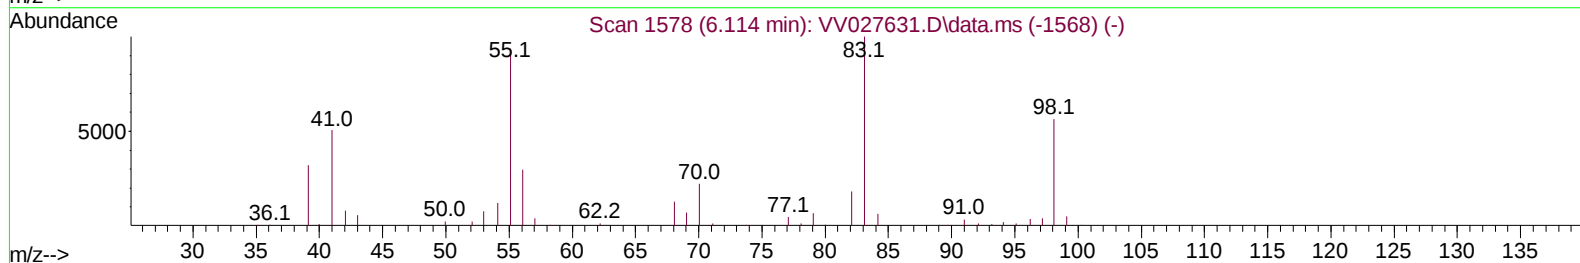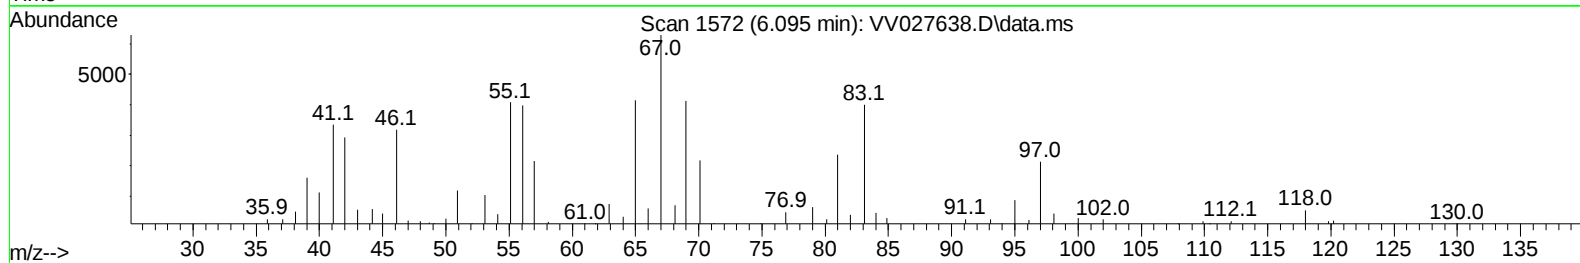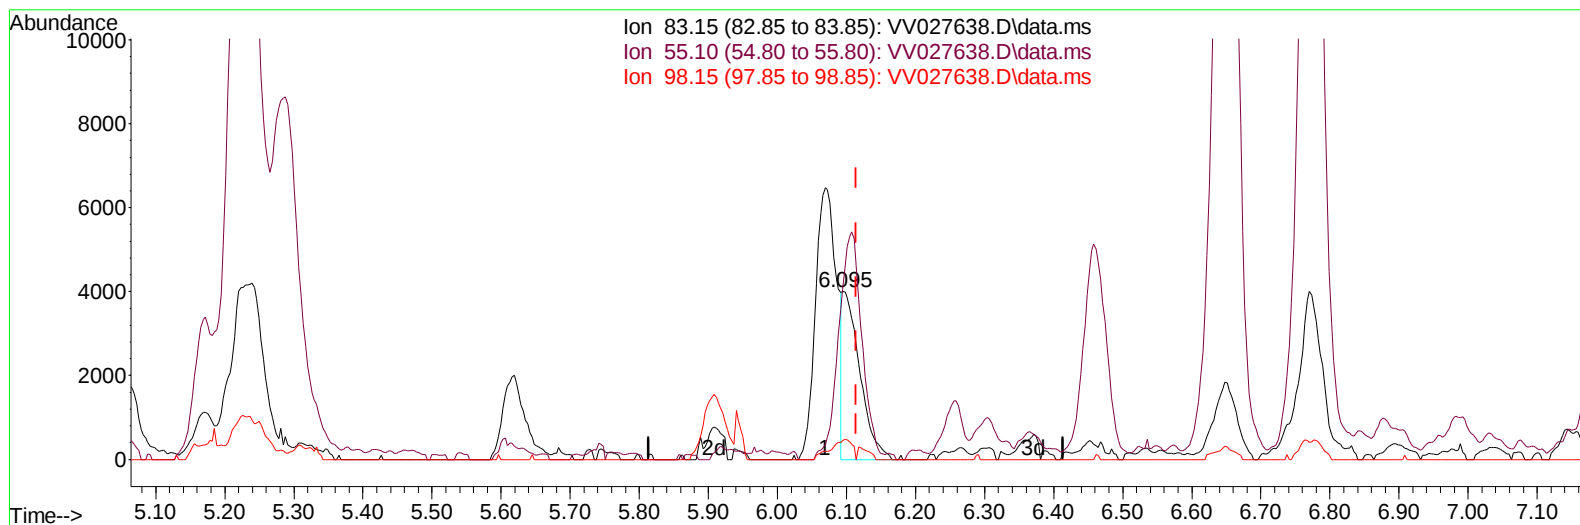

TIC: VV027638.D\data.ms

(35) Methylcyclohexane (T)

6.095min (-0.019) 0.33 ug/L m

response 7068

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	82.50	0.00#
98.15	46.10	14.77#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027638.D
 Acq On : 01 Sep 2022 00:42
 Operator : SY/MD
 Sample : N4366-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 01 04:16:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	153931	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	145339	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59294	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	48552	2.903	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	58.000%	
7) Chloroethane-d5	1.561	69	39692	2.837	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	56.800%#	
11) 1,1-Dichloroethene-d2	2.101	63	74444	2.275	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	45.400%#	
20) 2-Butanone-d5	3.905	46	82554	29.198	ug/L	-0.04
Spiked Amount 50.000	Range 40	- 130	Recovery	=	58.400%	
24) Chloroform-d	4.346	84	92162	2.745	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	55.000%#	
26) 1,2-Dichloroethane-d4	5.031	65	46197	3.072	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	61.400%#	
32) Benzene-d6	5.047	84	182232	3.061	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	=	61.200%#	
36) 1,2-Dichloropropane-d6	6.069	67	56354	3.060	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	61.200%	
41) Toluene-d8	7.313	98	143467	2.783	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	55.600%#	
43) trans-1,3-Dichloroprop...	7.629	79	6792	1.197	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	24.000%#	
46) 2-Hexanone-d5	8.092	63	45870	21.502	ug/L	-0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	43.000%#	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33464	2.824	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	56.400%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	42678	3.215	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	64.400%#	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.307	62	9607	0.502	ug/L #	81
12) 1,1-Dichloroethene	2.111	96	1760	0.137	ug/L #	1
17) Methyl tert-butyl Ether	2.770	73	79093	2.882	ug/L #	1
18) trans-1,2-Dichloroethene	2.754	96	427887	29.381	ug/L	99
22) cis-1,2-Dichloroethene	3.905	96	316589	21.781	ug/L	96
30) Cyclohexane	4.670	56	9427	0.445	ug/L	93
33) Benzene	5.105	78	16024	0.283	ug/L	100
34) Trichloroethene	5.912	95	98982	7.103	ug/L	98
35) Methylcyclohexane	6.095	83	7068m	0.327	ug/L	
47) Tetrachloroethene	7.976	164	4316	0.382	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027638.D
Acq On : 01 Sep 2022 00:42
Operator : SY/MD
Sample : N4366-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E76

Manual IntegrationsAPPROVED

Quant Time: Sep 01 04:16:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:22:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

