




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027647.D
 Acq On : 01 Sep 2022 04:22
 Operator : SY/MD
 Sample : N4418-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWH7

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

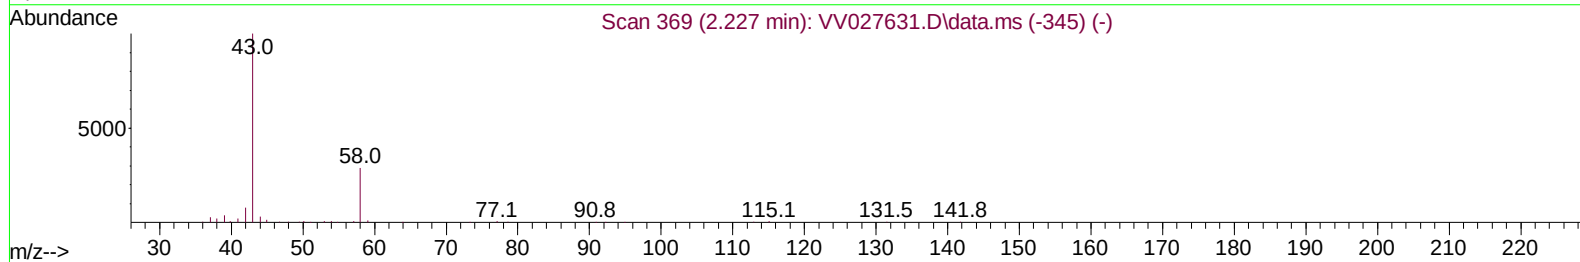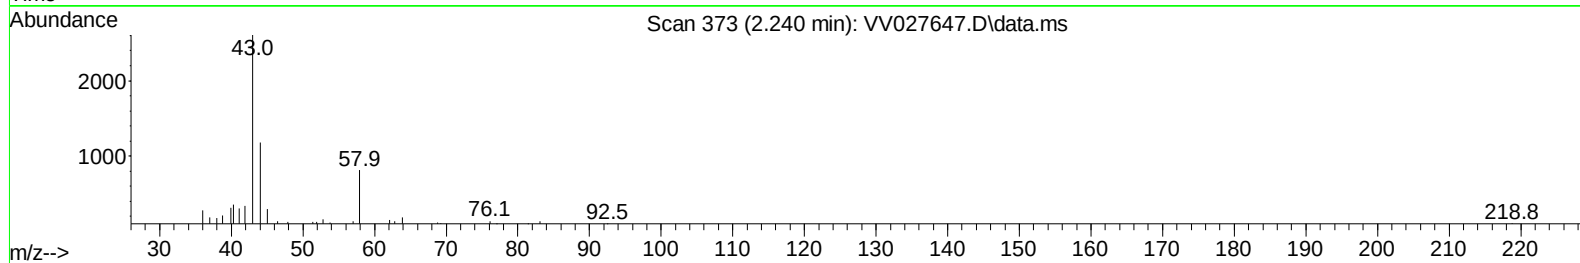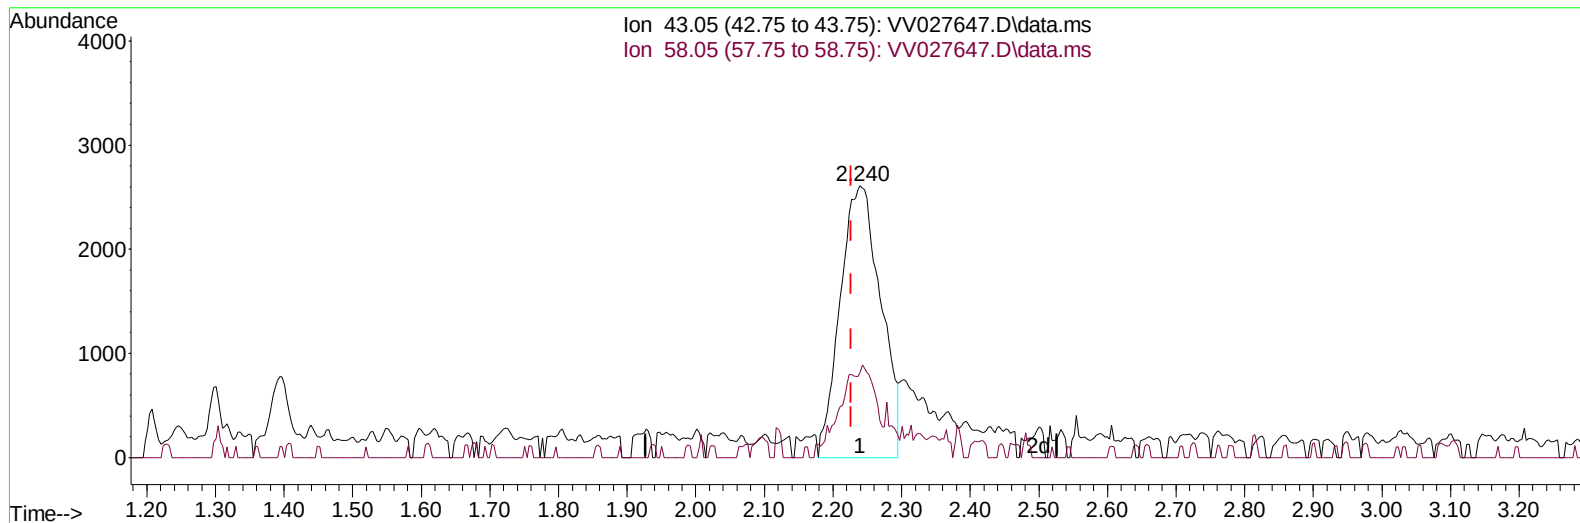

TIC: VV027647.D\data.ms

(13) Acetone (T)

2.240min (+ 0.013) 5.10 ug/L

response 10701

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	10.74
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027647.D
 Acq On : 01 Sep 2022 04:22
 Operator : SY/MD
 Sample : N4418-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWH7

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

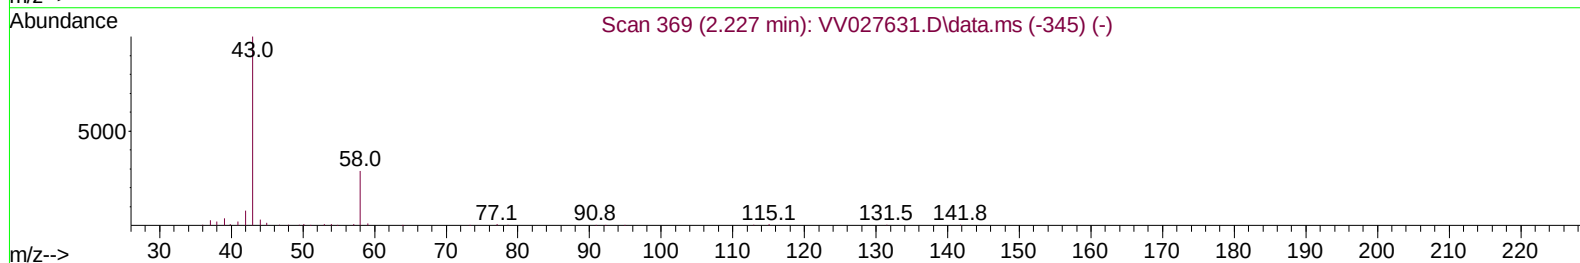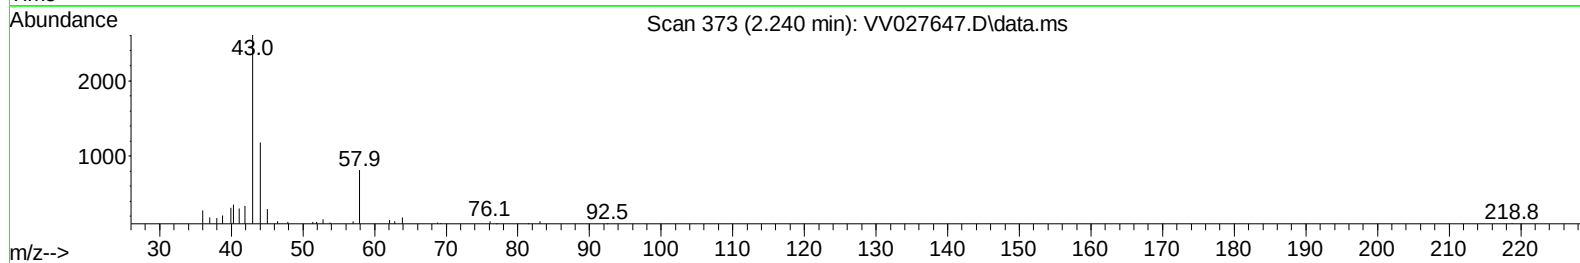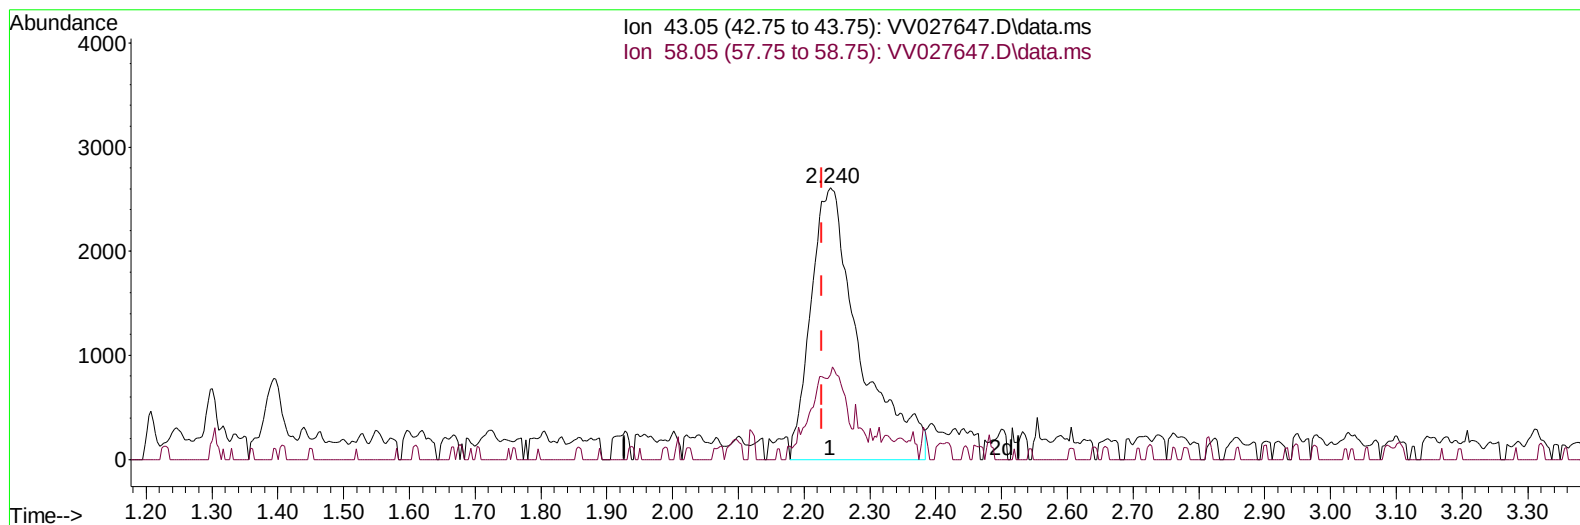

TIC: VV027647.D\data.ms

(13) Acetone (T)

2.240min (+ 0.013) 6.39 ug/L m

response 13411

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	8.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027647.D
 Acq On : 01 Sep 2022 04:22
 Operator : SY/MD
 Sample : N4418-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWH7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Quant Time: Sep 01 05:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.596	114	168909	5.000	ug/L	-0.01
28) Chlorobenzene-d5	8.860	117	127011	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	51343	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	69506	3.788	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	75.800%	
7) Chloroethane-d5	1.558	69	59109	3.850	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	77.000%	
11) 1,1-Dichloroethene-d2	2.098	63	103888	2.893	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	57.800%#	
20) 2-Butanone-d5	3.969	46	146553	47.238	ug/L	0.03
Spiked Amount 50.000	Range 40	- 130	Recovery	=	94.480%	
24) Chloroform-d	4.358	84	131775	3.577	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	=	71.600%	
26) 1,2-Dichloroethane-d4	5.030	65	71118	4.310	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.200%	
32) Benzene-d6	5.037	84	240596	4.625	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	6.059	67	79672	4.951	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	99.000%	
41) Toluene-d8	7.333	98	182637	4.054	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	7.641	79	21075	4.251	ug/L	0.02
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.000%	
46) 2-Hexanone-d5	8.117	63	69908	37.499	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	75.000%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	44994	4.345	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	86.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	59211	5.151	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	103.000%	
Target Compounds						Qvalue
13) Acetone	2.240	43	13411m	6.388	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027647.D
Acq On : 01 Sep 2022 04:22
Operator : SY/MD
Sample : N4418-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWH7

Manual IntegrationsAPPROVED

Quant Time: Sep 01 05:04:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:22:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

