




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027651.D
 Acq On : 01 Sep 2022 06:00
 Operator : SY/MD
 Sample : N4400-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA4

Manual IntegrationsAPPROVED

Quant Time: Sep 01 07:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

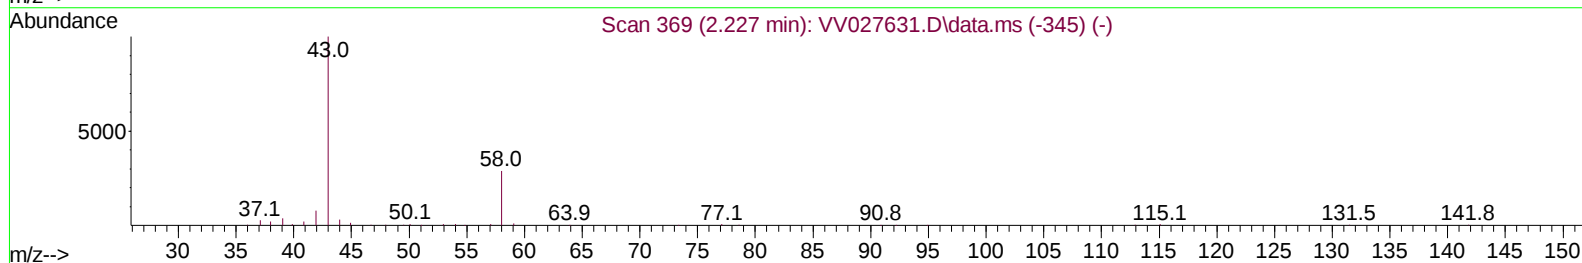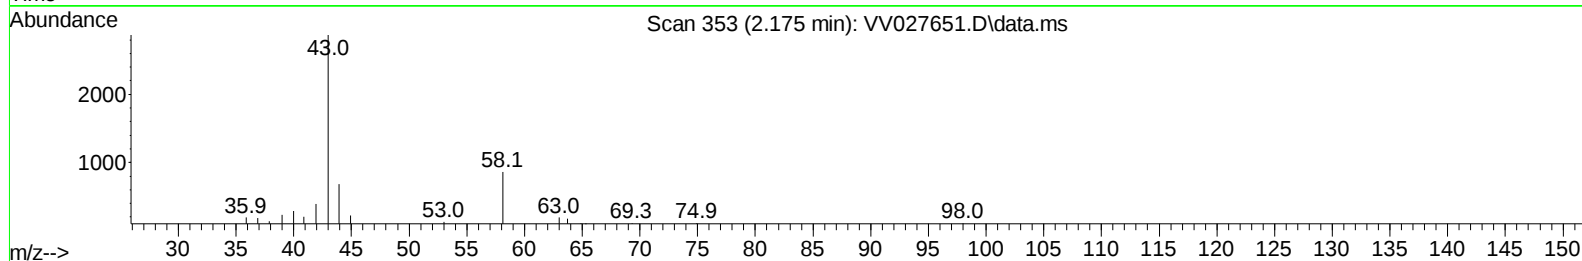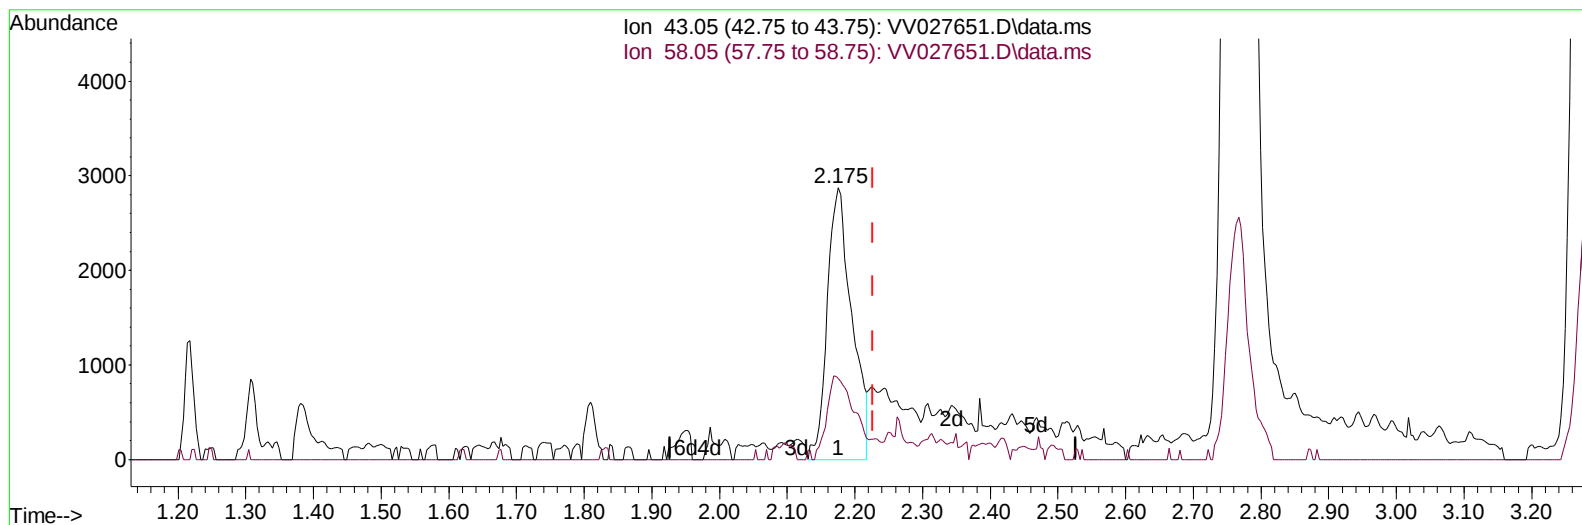

TIC: VV027651.D\data.ms

(13) Acetone (T)

2.175min (-0.051) 4.43 ug/L

response 7250

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	34.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027651.D
 Acq On : 01 Sep 2022 06:00
 Operator : SY/MD
 Sample : N4400-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA4

Manual IntegrationsAPPROVED

Quant Time: Sep 01 07:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

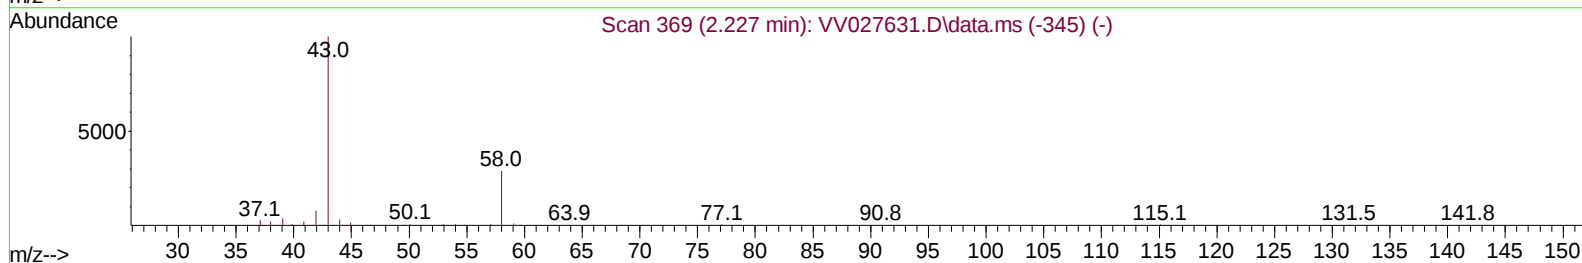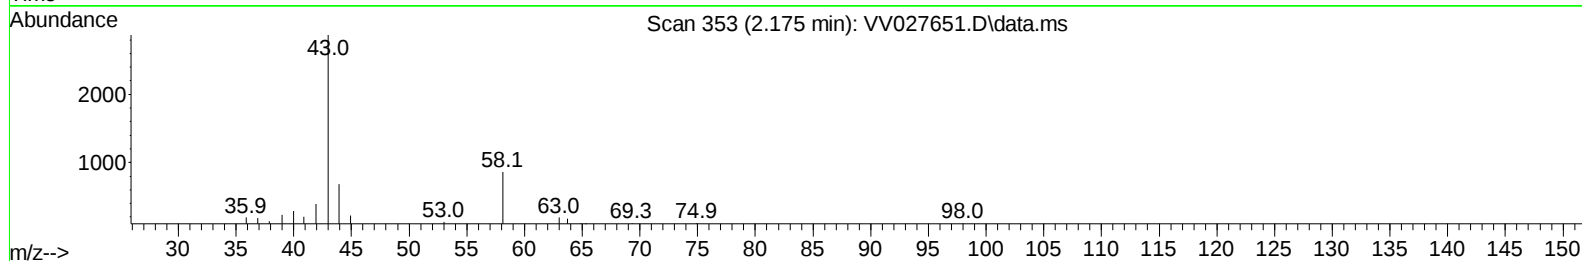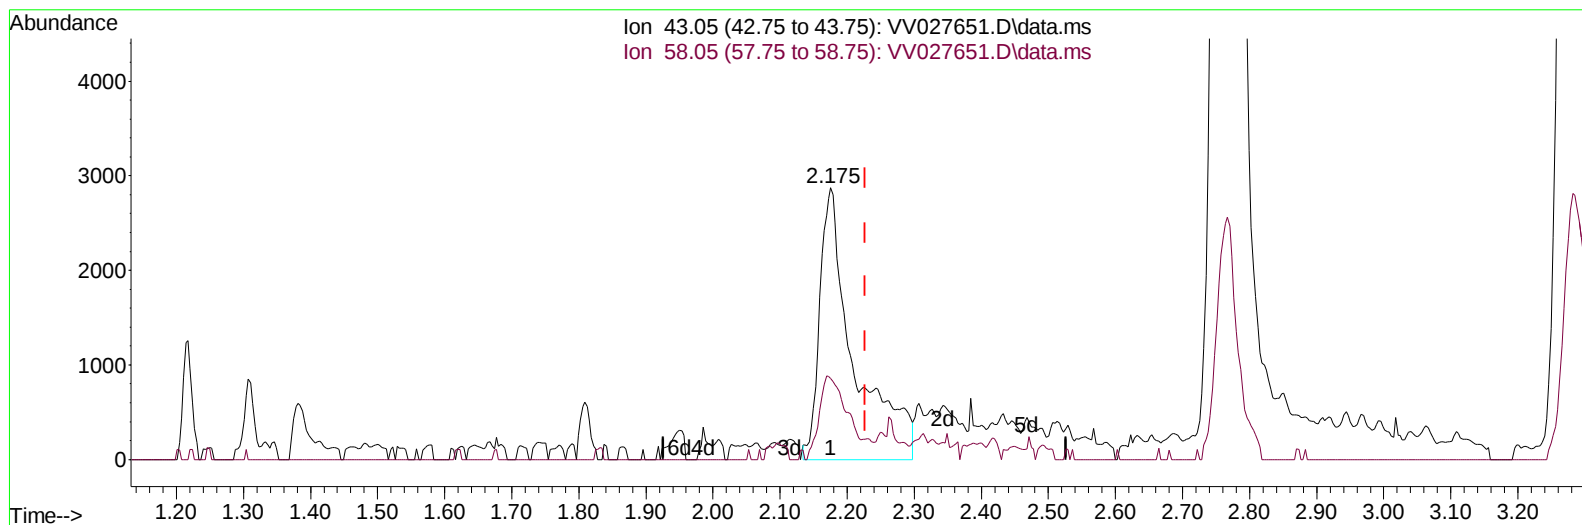

TIC: VV027651.D\data.ms

(13) Acetone (T)

2.175min (-0.051) 6.23 ug/L m

response 10186

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	24.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027651.D
 Acq On : 01 Sep 2022 06:00
 Operator : SY/MD
 Sample : N4400-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA4

Manual IntegrationsAPPROVED

Quant Time: Sep 01 07:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	131600	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	134811	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	54561	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	69340	4.850	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	97.000%	
7) Chloroethane-d5	1.568	69	60709	5.075	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	101.600%	
11) 1,1-Dichloroethene-d2	2.108	63	104842	3.747	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	75.000%	
20) 2-Butanone-d5	3.886	46	72113	29.834	ug/L	-0.06
Spiked Amount 50.000	Range 40	- 130	Recovery	=	59.660%	
24) Chloroform-d	4.346	84	133691	4.658	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.200%	
26) 1,2-Dichloroethane-d4	5.031	65	61486	4.782	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	95.600%	
32) Benzene-d6	5.047	84	246909	4.471	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	=	89.400%	
36) 1,2-Dichloropropane-d6	6.066	67	74510	4.362	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	87.200%	
41) Toluene-d8	7.314	98	190608	3.986	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	79.800%	
43) trans-1,3-Dichloroprop...	7.622	79	20338	3.865	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	77.400%	
46) 2-Hexanone-d5	8.088	63	78281	39.561	ug/L	-0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	79.120%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46804	4.258	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	85.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	68366	5.597	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	112.000%	
Target Compounds						
						Qvalue
5) Vinyl chloride	1.311	62	81109	4.962	ug/L	97
13) Acetone	2.175	43	10186m	6.228	ug/L	
14) Carbon disulfide	2.294	76	40417	1.164	ug/L	98
17) Methyl tert-butyl Ether	2.767	73	339281	14.458	ug/L	99
18) trans-1,2-Dichloroethene	2.761	96	5817	0.467	ug/L	98
22) cis-1,2-Dichloroethene	3.905	96	406484	32.711	ug/L	94
27) 1,2-Dichloroethane	5.150	62	2289	0.164	ug/L #	78
33) Benzene	5.101	78	30202	0.574	ug/L	100
34) Trichloroethene	5.915	95	14270	1.104	ug/L	95
42) Toluene	7.394	91	14638	0.279	ug/L	99
47) Tetrachloroethene	7.976	164	1744	0.166	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027651.D
Acq On : 01 Sep 2022 06:00
Operator : SY/MD
Sample : N4400-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA4

Manual IntegrationsAPPROVED

Quant Time: Sep 01 07:01:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:22:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

