




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027659.D
 Acq On : 01 Sep 2022 10:39
 Operator : SY/MD
 Sample : N4400-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG6

Manual IntegrationsAPPROVED

Quant Time: Sep 01 23:15:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 07:36:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

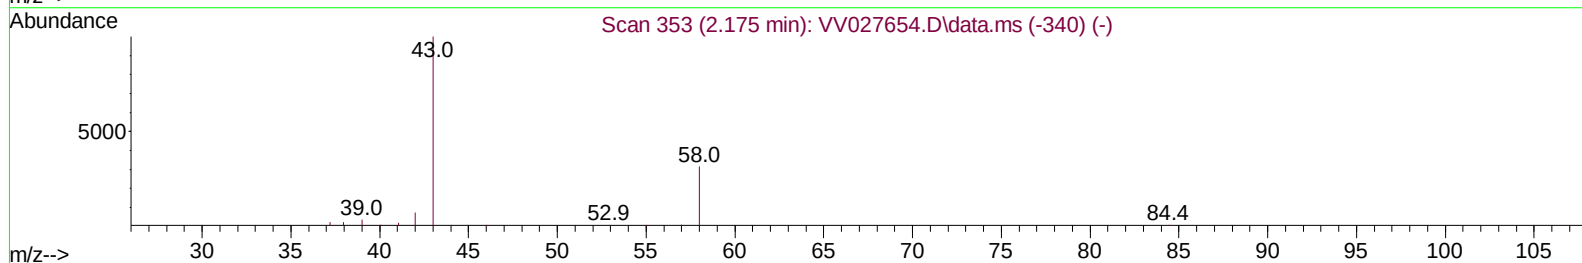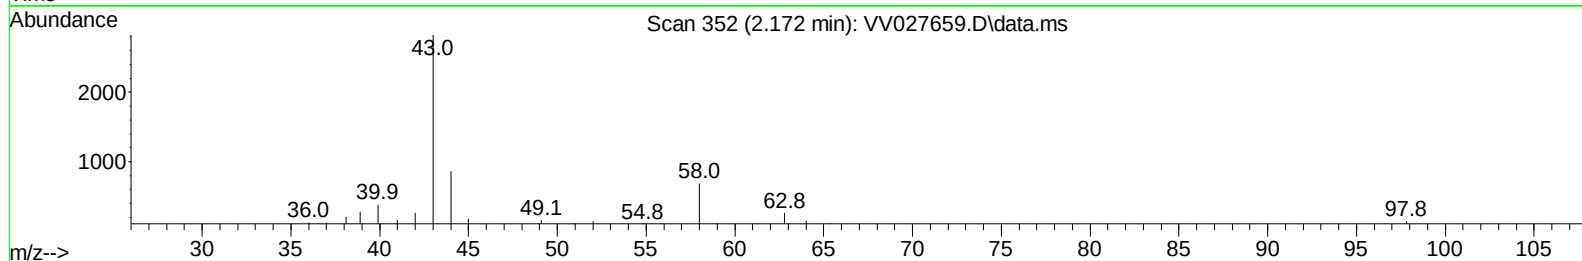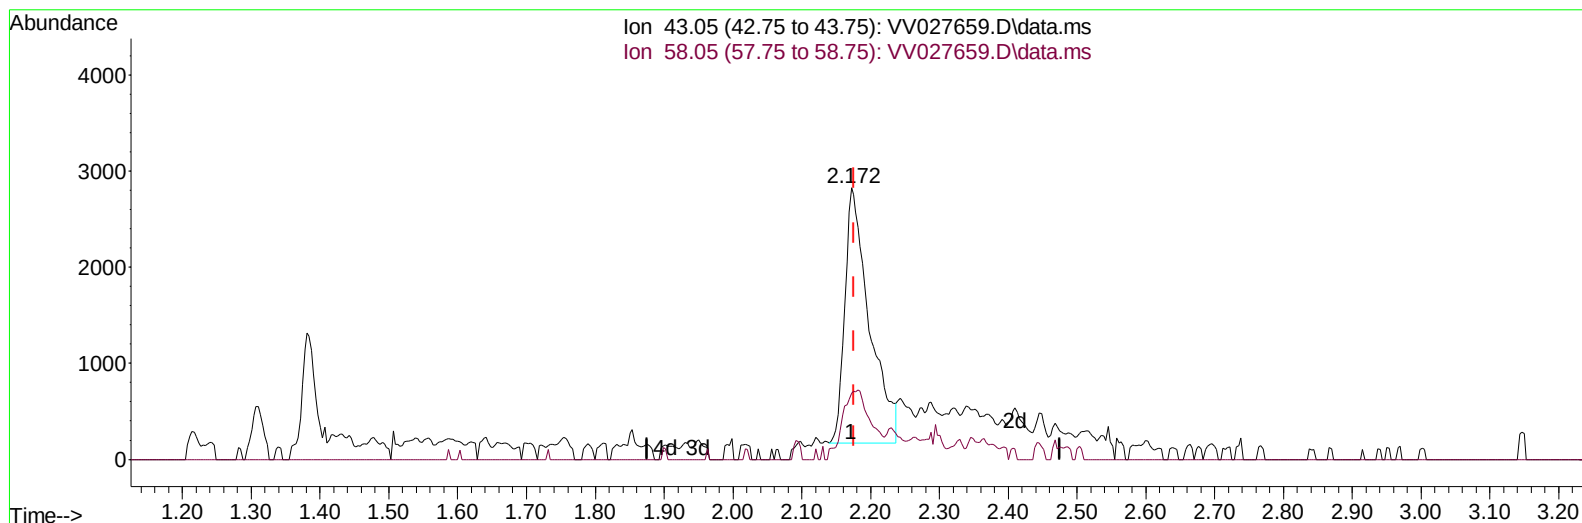

TIC: VV027659.D\data.ms

(13) Acetone (T)

2.172min (-0.003) 4.18 ug/L

response 6591

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	31.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027659.D
 Acq On : 01 Sep 2022 10:39
 Operator : SY/MD
 Sample : N4400-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG6

Manual IntegrationsAPPROVED

Quant Time: Sep 01 23:15:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 07:36:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

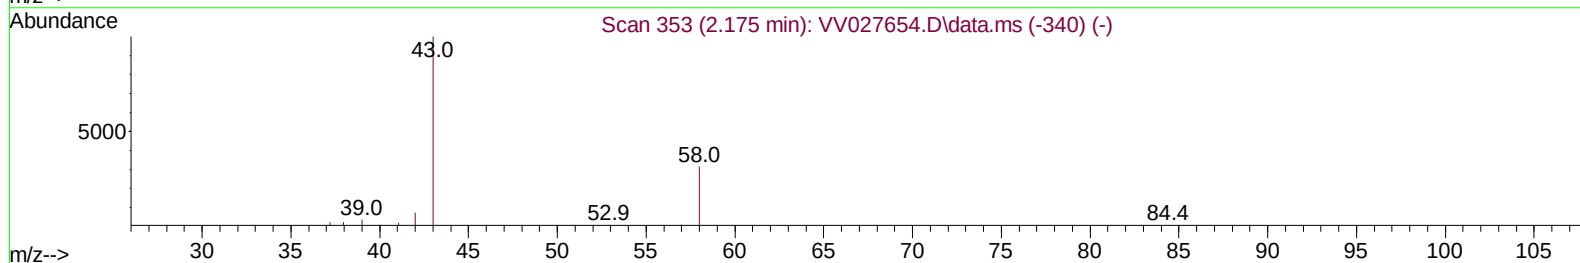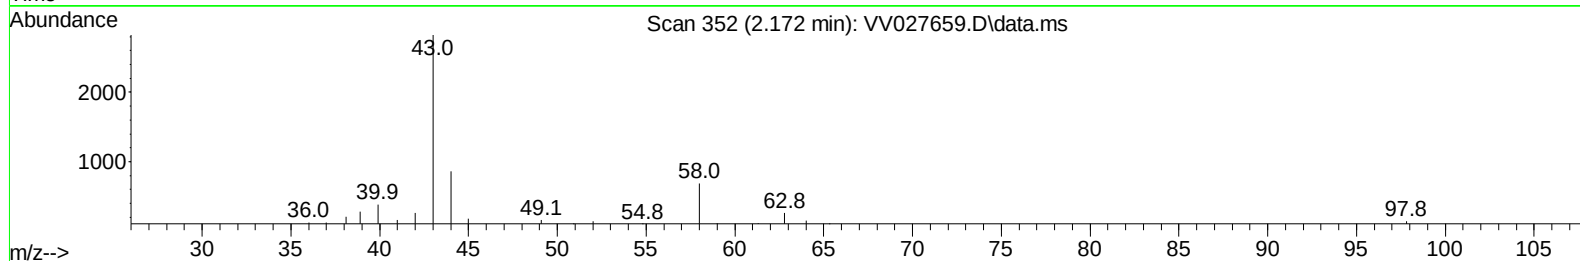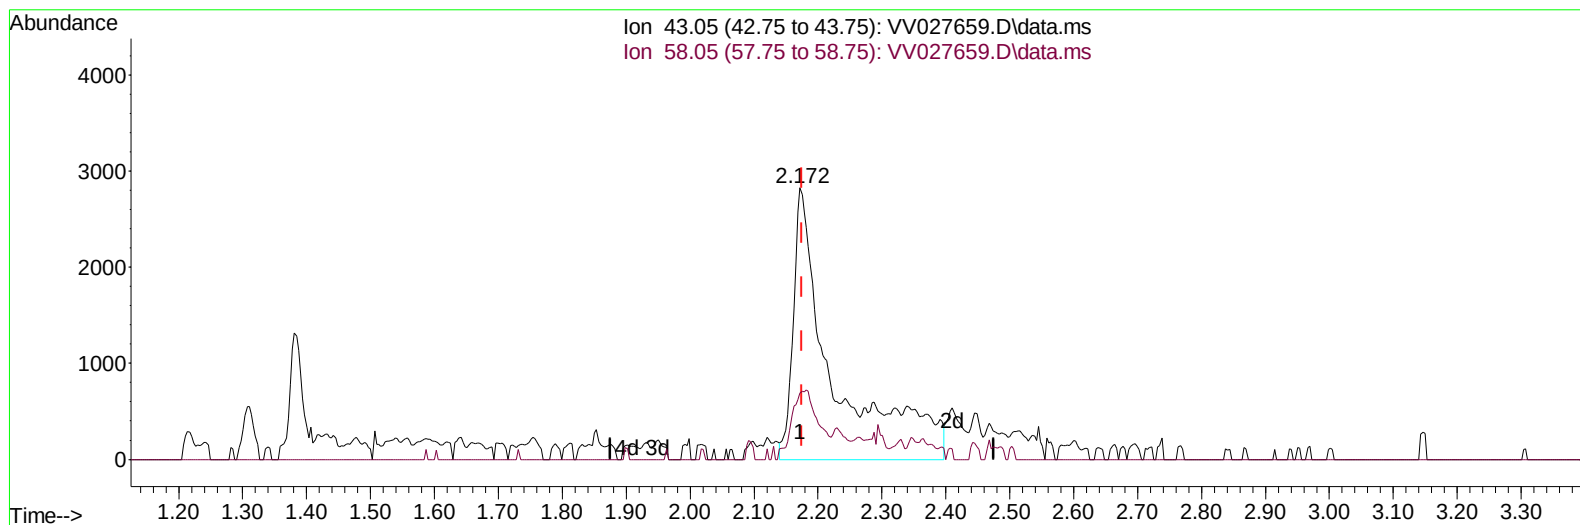

TIC: VV027659.D\data.ms

(13) Acetone (T)

2.172min (-0.003) 7.82 ug/L m

response 12319

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	19.20	16.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027659.D
 Acq On : 01 Sep 2022 10:39
 Operator : SY/MD
 Sample : N4400-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG6

Manual IntegrationsAPPROVED

Quant Time: Sep 01 23:15:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 07:36:37 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		126734	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		126132	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		53792	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		67428	4.897	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.000%	
7) Chloroethane-d5	1.568	69		60457	5.248	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.000%	
11) 1,1-Dichloroethene-d2	2.108	63		105089	3.900	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.000%	
20) 2-Butanone-d5	3.895	46		73645	31.637	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	63.280%	
24) Chloroform-d	4.346	84		133090	4.815	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.030	65		59610	4.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%	
32) Benzene-d6	5.047	84		247555	4.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.066	67		75516	4.725	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%	
41) Toluene-d8	7.313	98		194384	4.345	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	7.625	79		19987	4.060	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%	
46) 2-Hexanone-d5	8.088	63		78639	42.476	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.960%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		43767	4.256	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		63644	5.285	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%	
Target Compounds							
13) Acetone	2.172	43		12319m	7.821	ug/L	
14) Carbon disulfide	2.294	76		5926	0.177	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027659.D
Acq On : 01 Sep 2022 10:39
Operator : SY/MD
Sample : N4400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBVG6

Manual IntegrationsAPPROVED

Quant Time: Sep 01 23:15:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 07:36:37 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/02/2022
Supervised By :Mahesh Dadoda 09/02/2022

