

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027614.D
 Acq On : 31 Aug 2022 12:07
 Operator : SY/MD
 Sample : N4367-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 01 02:34:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:33:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	141267	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	141540	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	58787	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44133	4.390	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.800%	
7) Chloroethane-d5	1.568	69	37511	5.098	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.000%	
11) 1,1-Dichloroethene-d2	2.108	63	65144	2.779	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.600%#	
20) 2-Butanone-d5	3.896	46	59802	47.795	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.600%	
24) Chloroform-d	4.346	84	93824	4.667	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	5.031	65	44476	5.114	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.050	84	168724	4.304	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	6.069	67	54983	4.824	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.317	98	122796	3.469	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.400%#	
43) trans-1,3-Dichloroprop...	7.625	79	16005	4.101	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.092	63	62661	48.776	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.560%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37345	5.145	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	42468	4.873	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	4016	0.249	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027614.D
Acq On : 31 Aug 2022 12:07
Operator : SY/MD
Sample : N4367-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 01 02:34:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:33:10 2022
Response via : Initial Calibration

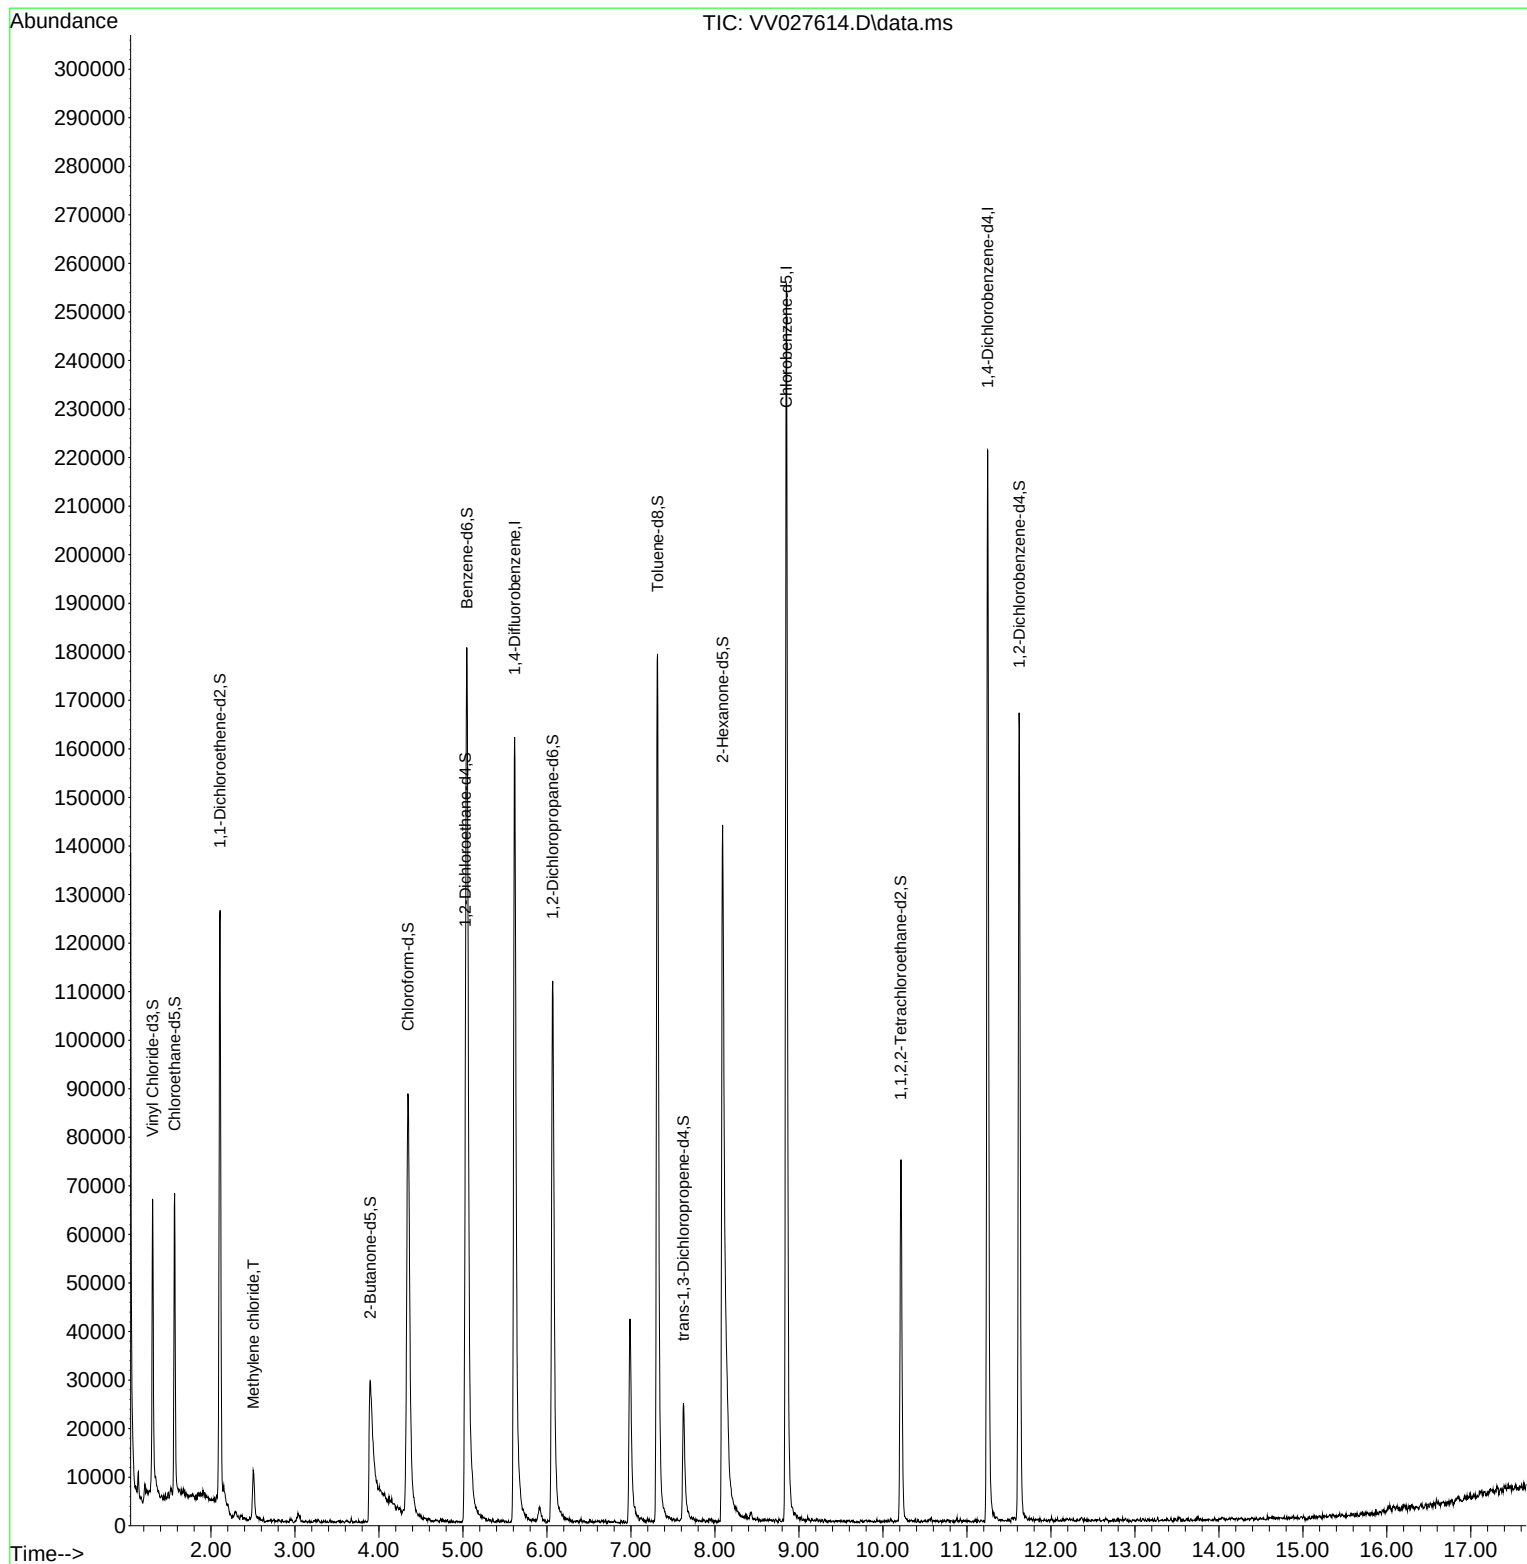

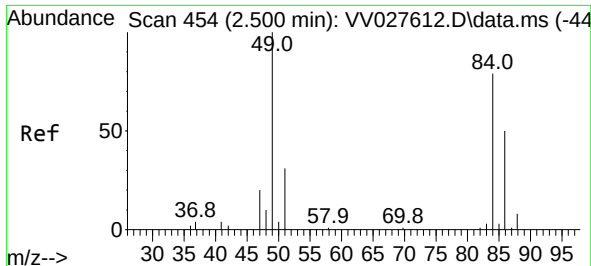

#16
Methylene chloride
Concen: 0.249 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV027614.D
Acq: 31 Aug 2022 12:07

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4016
Ion Ratio Lower Upper
84 100
86 60.7 44.0 81.6
49 118.3 89.4 166.0

