

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083122\
 Data File : VW027647.D
 Acq On : 01 Sep 2022 04:22
 Operator : SY/MD
 Sample : N4418-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWH7

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/01/2022
 Supervised By :Mahesh Dadoda 09/02/2022

Quant Time: Sep 01 05:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 02:22:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.596	114	168909	5.000	ug/L	-0.01
28) Chlorobenzene-d5	8.860	117	127011	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	51343	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	69506	3.788	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.800%
7) Chloroethane-d5	1.558	69	59109	3.850	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.000%
11) 1,1-Dichloroethene-d2	2.098	63	103888	2.893	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.800%#
20) 2-Butanone-d5	3.969	46	146553	47.238	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.480%
24) Chloroform-d	4.358	84	131775	3.577	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.600%
26) 1,2-Dichloroethane-d4	5.030	65	71118	4.310	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
32) Benzene-d6	5.037	84	240596	4.625	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.059	67	79672	4.951	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.333	98	182637	4.054	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	7.641	79	21075	4.251	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.117	63	69908	37.499	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.000%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	44994	4.345	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	59211	5.151	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds					Qvalue	
13) Acetone	2.240	43	13411m	6.388	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027647.D
Acq On : 01 Sep 2022 04:22
Operator : SY/MD
Sample : N4418-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBWH7

Quant Time: Sep 01 05:04:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 02:22:45 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

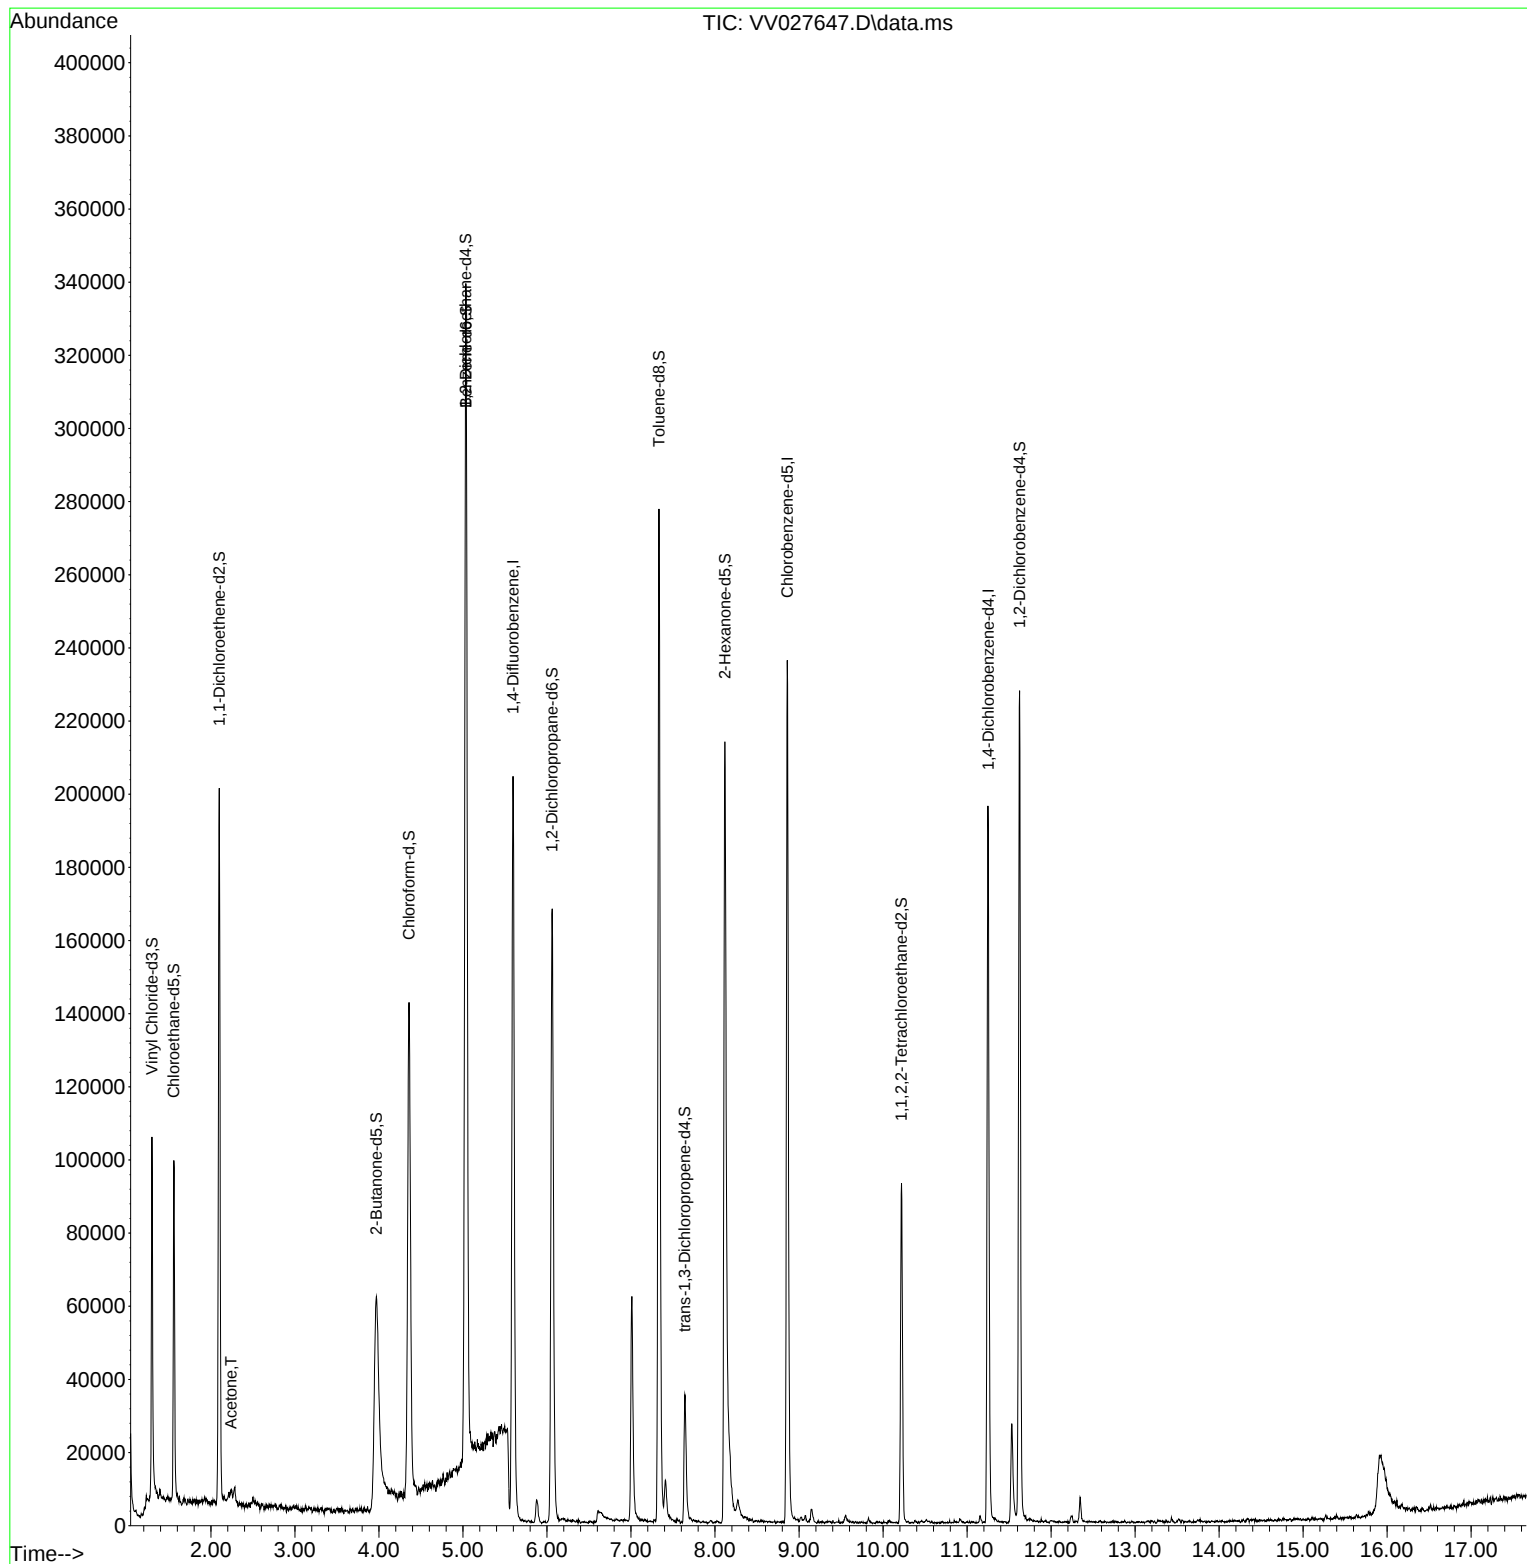

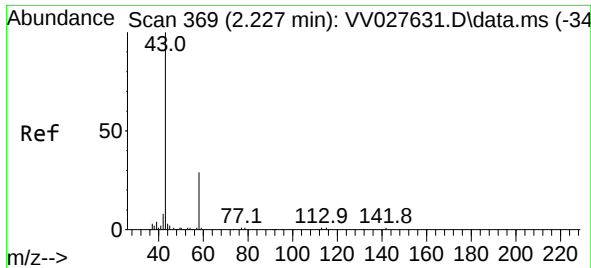

#13
Acetone
Concen: 6.388 ug/L m
RT: 2.240 min Scan# 31
Delta R.T. 0.013 min
Lab File: VV027647.D
Acq: 01 Sep 2022 04:22

Instrument :
MSVOA_V
ClientSampleId :
DBWH7

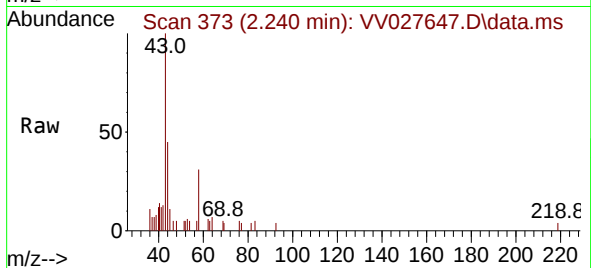

Tgt Ion: 43 Resp: 1341
Ion Ratio Lower Upper
43 100
58 8.6 0.0 38.4

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 09/01/2022
Supervised By :Mahesh Dadoda 09/02/2022

