

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027655.D
 Acq On : 01 Sep 2022 08:02
 Operator : SY/MD
 Sample : VV0831WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Quant Time: Sep 01 08:18:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 01 07:36:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	139693	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	130791	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52118	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	73661	4.854	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.571	69	59928	4.720	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.400%
11) 1,1-Dichloroethene-d2	2.111	63	106803	3.596	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.969	46	146330	57.030	ug/L	0.08
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.060%
24) Chloroform-d	4.349	84	131059	4.302	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.037	65	72439	5.308	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.043	84	255125	4.762	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	6.079	67	79839	4.818	ug/L	0.01
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.400%
41) Toluene-d8	7.326	98	193746	4.176	ug/L	0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.635	79	20608	4.037	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	8.111	63	77672	40.459	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.920%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46395	4.351	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	59167	5.071	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	5856	0.398	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027655.D
Acq On : 01 Sep 2022 08:02
Operator : SY/MD
Sample : VV0831WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Time: Sep 01 08:18:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 01 07:36:37 2022
Response via : Initial Calibration

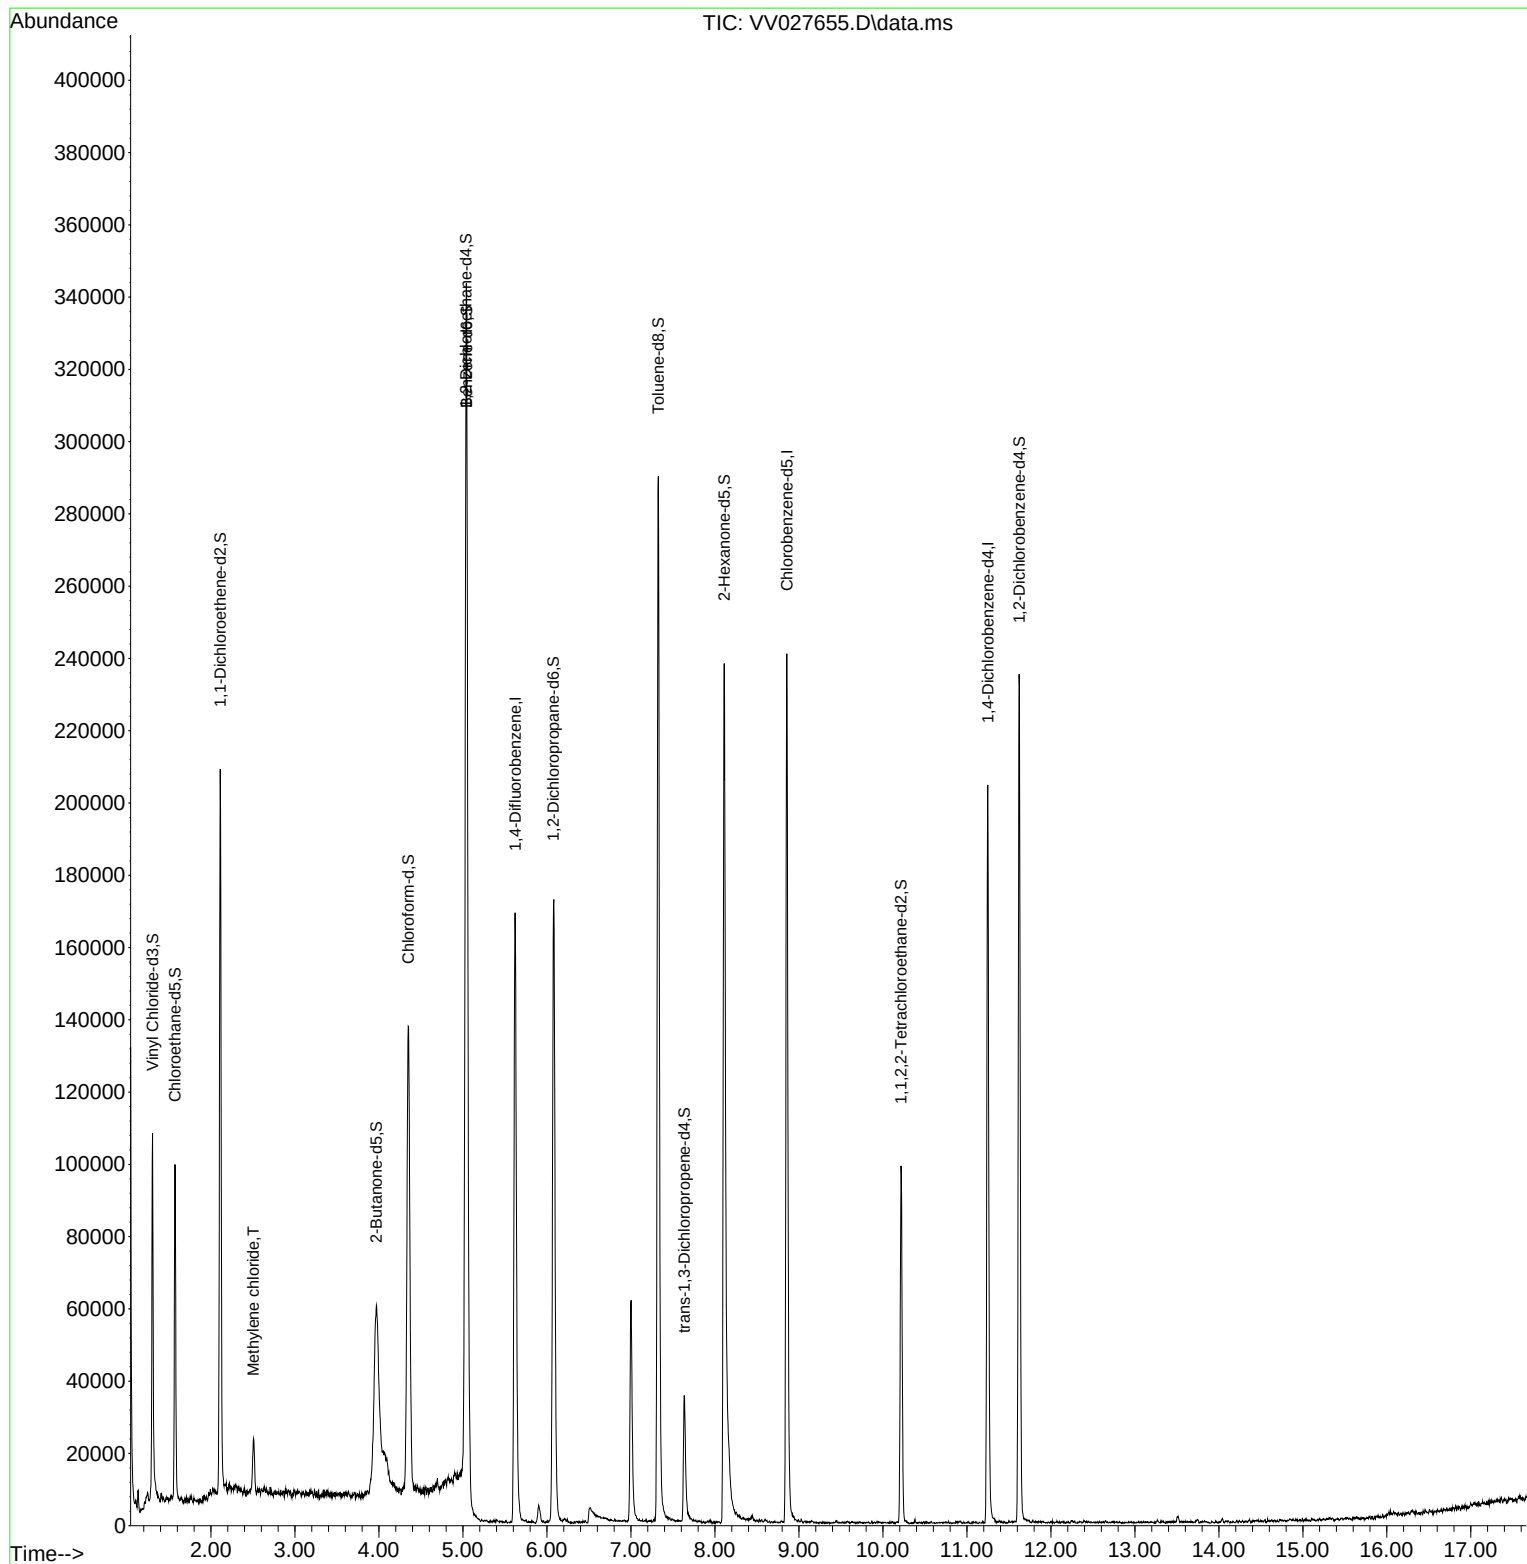

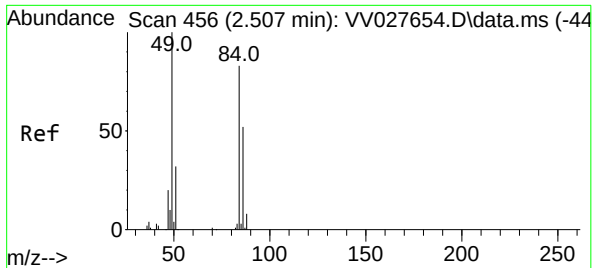

#16
Methylene chloride
Concen: 0.398 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV027655.D
Acq: 01 Sep 2022 08:02

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Tgt Ion: 84 Resp: 5856
Ion Ratio Lower Upper
84 100
86 61.4 43.9 81.5
49 136.5 92.5 171.7

