

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027633.D
 Acq On : 31 Aug 2022 22:40
 Operator : SY/MD
 Sample : N4366-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E70

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	71	81	91	rBV	104315	114409	16.67%	2.352%
2	1.561	155	162	176	rVB	89686	100810	14.69%	2.073%
3	2.098	316	329	341	rBV	196022	282676	41.19%	5.812%
4	2.770	524	538	555	rBV2	67621	149726	21.82%	3.078%
5	3.902	880	890	927	rBV	43617	171721	25.02%	3.531%
6	4.342	1011	1027	1061	rBV	120576	322775	47.03%	6.636%
7	5.043	1226	1245	1286	rBV2	261766	686337	100.00%	14.111%
8	5.612	1412	1422	1456	rBV	137791	300247	43.75%	6.173%
9	5.905	1502	1513	1527	rVB9	4417	9806	1.43%	0.202%
10	6.066	1548	1563	1589	rBV	157306	341870	49.81%	7.029%
11	6.985	1835	1849	1869	rBV	57878	116169	16.93%	2.388%
12	7.313	1939	1951	1973	rBV	273363	497209	72.44%	10.222%
13	7.622	2037	2047	2061	rBV	36254	67275	9.80%	1.383%
14	8.091	2182	2193	2227	rBV	223835	488816	71.22%	10.050%
15	8.850	2417	2429	2451	rBV	221982	379362	55.27%	7.800%
16	10.214	2839	2853	2870	rBV	97828	157707	22.98%	3.242%
17	11.246	3163	3174	3196	rBV	187107	297079	43.28%	6.108%
18	11.622	3280	3291	3306	rBV	220188	353354	51.48%	7.265%
19	15.924	4613	4629	4630	rBV9	9341	17313	2.52%	0.356%
20	16.178	4701	4708	4716	rVB10	7117	9232	1.35%	0.190%




Sum of corrected areas: 4863893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027633.D
Acq On : 31 Aug 2022 22:40
Operator : SY/MD
Sample : N4366-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

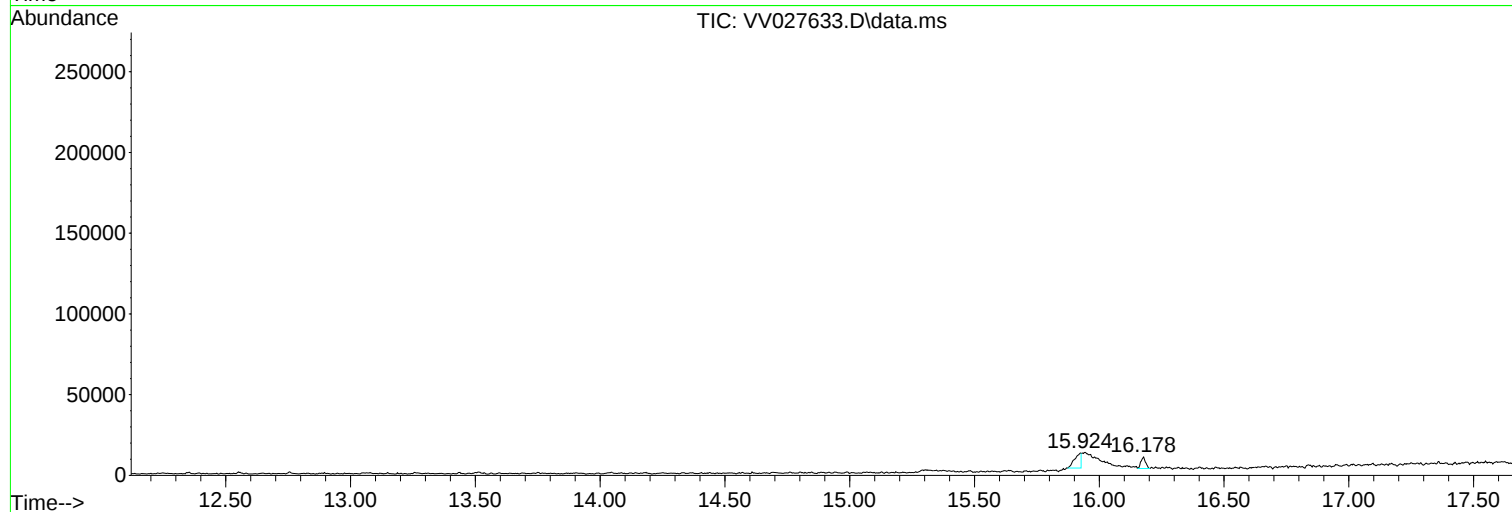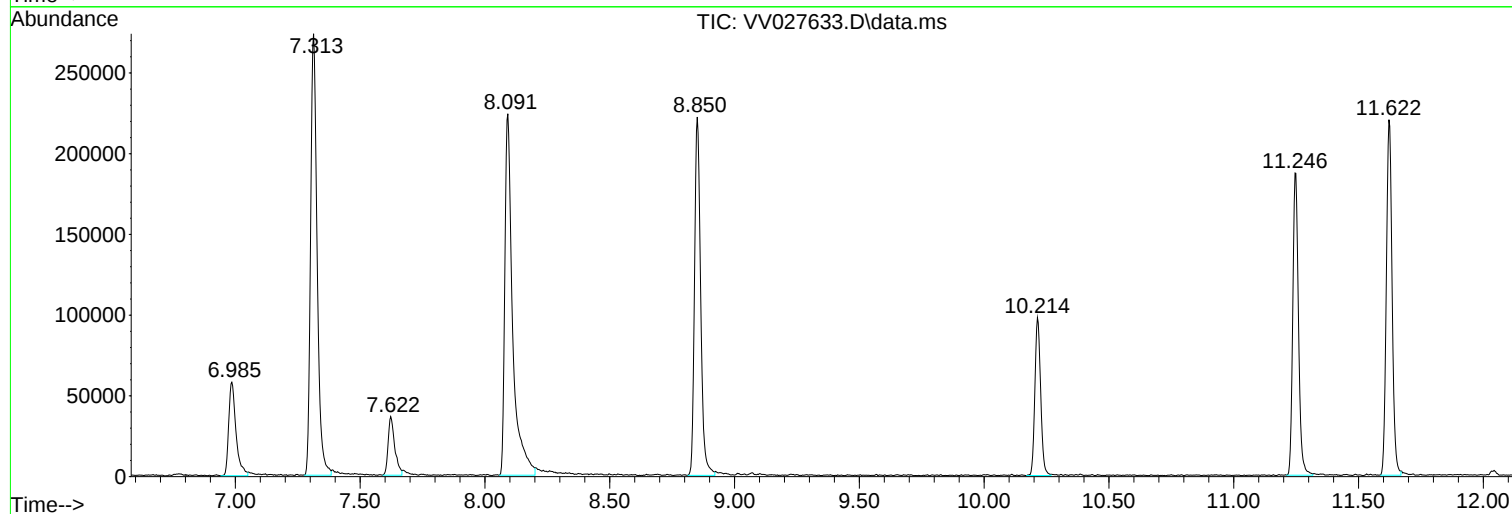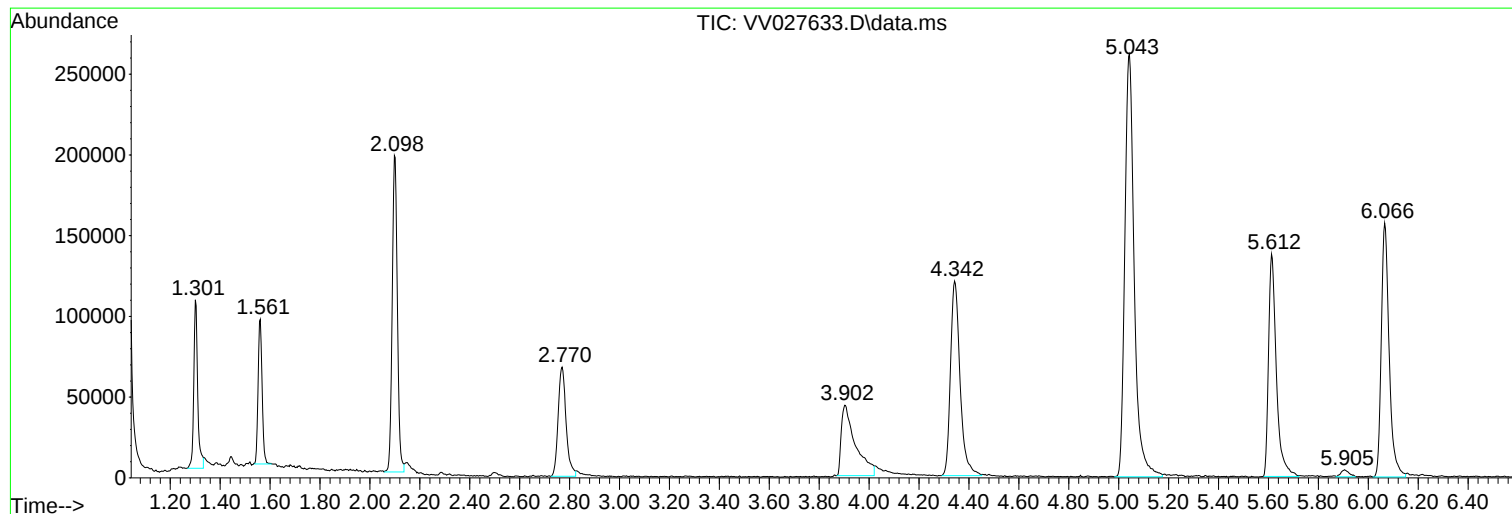

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027633.D
Acq On : 31 Aug 2022 22:40
Operator : SY/MD
Sample : N4366-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027633.D
Acq On : 31 Aug 2022 22:40
Operator : SY/MD
Sample : N4366-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc