

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027636.D
 Acq On : 31 Aug 2022 23:53
 Operator : SY/MD
 Sample : N4366-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	72	80	92	rBV	97353	110165	15.78%	2.151%
2	1.561	154	162	176	rBV	89510	103252	14.79%	2.016%
3	2.098	318	329	340	rBV	194393	277008	39.69%	5.407%
4	2.773	524	539	554	rBV	62088	138541	19.85%	2.704%
5	3.947	881	904	937	rBV2	44519	204543	29.30%	3.993%
6	4.339	1009	1026	1054	rBV	130776	328462	47.06%	6.412%
7	5.037	1228	1243	1275	rBV2	286807	698009	100.00%	13.626%
8	5.612	1410	1422	1458	rBV	144104	309903	44.40%	6.050%
9	5.911	1501	1515	1530	rBV8	16845	40283	5.77%	0.786%
10	6.066	1550	1563	1594	rBV	162730	350826	50.26%	6.848%
11	6.985	1836	1849	1873	rBV	59658	118079	16.92%	2.305%
12	7.310	1939	1950	1975	rBV	272366	503867	72.19%	9.836%
13	7.622	2037	2047	2068	rBV2	34882	69229	9.92%	1.351%
14	7.972	2145	2156	2173	rVB	85222	149105	21.36%	2.911%
15	8.095	2184	2194	2232	rBV	224338	509191	72.95%	9.940%
16	8.850	2415	2429	2450	rBV	231717	388850	55.71%	7.591%
17	10.214	2840	2853	2871	rBV	97564	155484	22.28%	3.035%
18	11.246	3162	3174	3197	rBV	190903	305807	43.81%	5.970%
19	11.622	3278	3291	3313	rBV	229821	362118	51.88%	7.069%




Sum of corrected areas: 5122722

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027636.D
Acq On : 31 Aug 2022 23:53
Operator : SY/MD
Sample : N4366-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

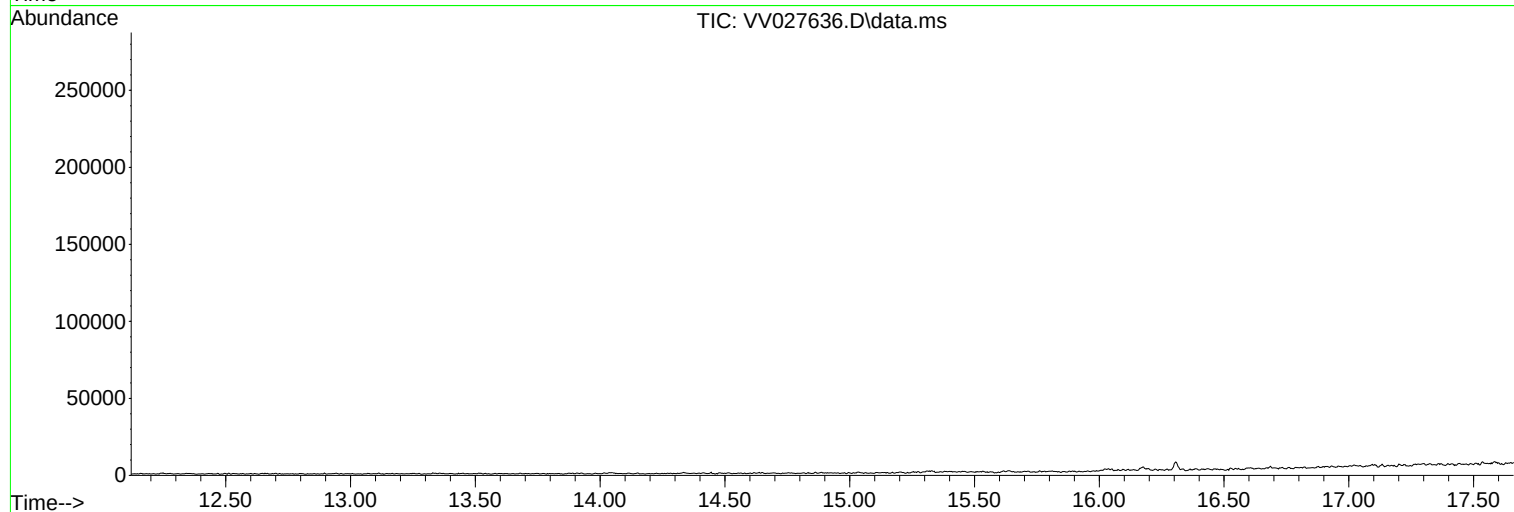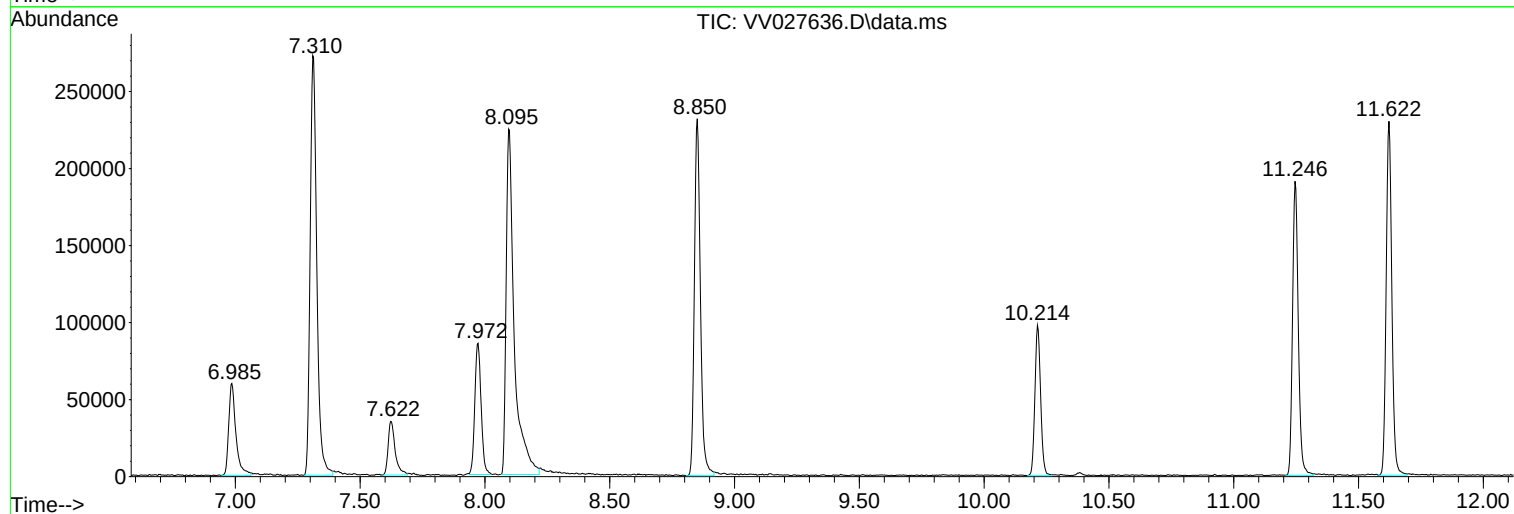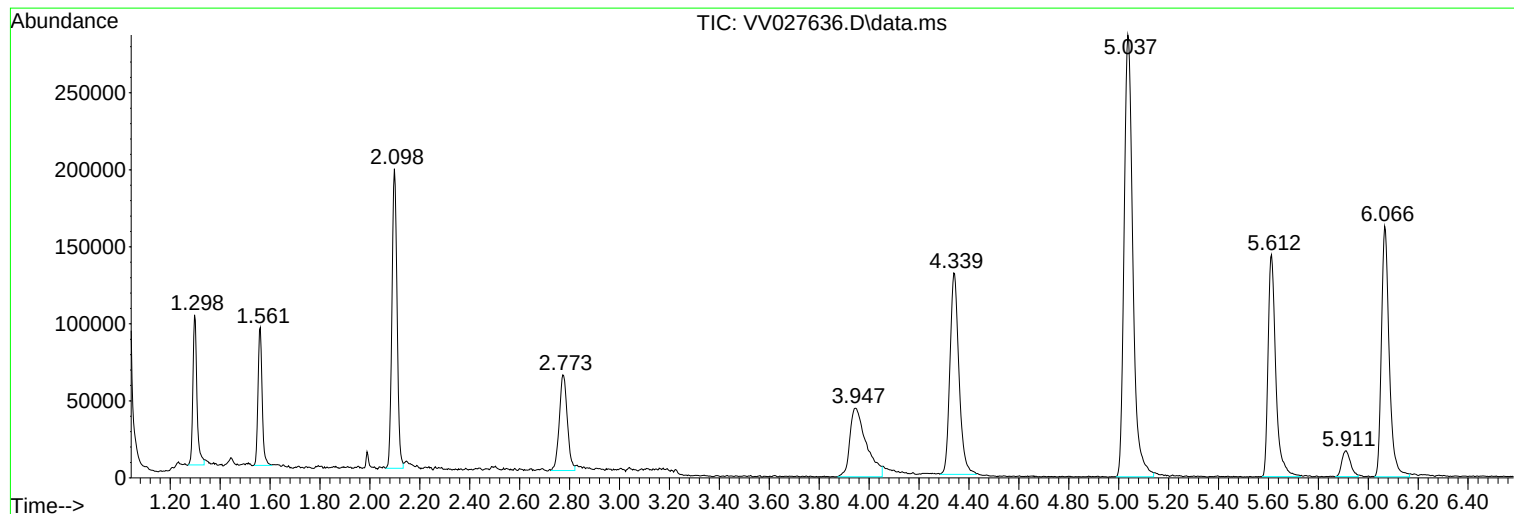

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027636.D
Acq On : 31 Aug 2022 23:53
Operator : SY/MD
Sample : N4366-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027636.D
Acq On : 31 Aug 2022 23:53
Operator : SY/MD
Sample : N4366-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
