

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027637.D
 Acq On : 01 Sep 2022 00:18
 Operator : SY/MD
 Sample : N4366-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E74

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	72	80	92	rBV	57823	64955	14.38%	1.680%
2	1.442	120	125	136	rBV10	5197	6438	1.42%	0.166%
3	1.561	154	162	171	rBV	57547	66615	14.74%	1.723%
4	2.098	320	329	340	rBV	117218	164312	36.37%	4.249%
5	2.291	385	389	397	rVB7	3864	6107	1.35%	0.158%
6	2.497	445	453	462	rBV6	3003	4746	1.05%	0.123%
7	2.773	523	539	557	rBV2	63062	143625	31.79%	3.714%
8	3.934	882	900	935	rBV2	30228	133557	29.56%	3.454%
9	4.346	1011	1028	1058	rVB	85250	220936	48.90%	5.713%
10	5.043	1229	1245	1272	rBV2	180172	451835	100.00%	11.684%
11	5.613	1411	1422	1449	rBV	148733	321441	71.14%	8.312%
12	5.915	1503	1516	1530	rBV8	15110	35179	7.79%	0.910%
13	6.066	1549	1563	1586	rBV	106862	233399	51.66%	6.035%
14	6.989	1840	1850	1869	rBV	32755	66258	14.66%	1.713%
15	7.313	1939	1951	1972	rBV	168847	307675	68.09%	7.956%
16	7.625	2037	2048	2068	rBV3	19106	38933	8.62%	1.007%
17	7.973	2146	2156	2172	rVB2	61669	106234	23.51%	2.747%
18	8.092	2182	2193	2227	rBV	151128	362145	80.15%	9.365%
19	8.850	2416	2429	2463	rBV	240239	405955	89.85%	10.498%
20	10.214	2839	2853	2867	rBV	69308	113680	25.16%	2.940%
21	11.246	3163	3174	3193	rBV	200886	317112	70.18%	8.200%
22	11.538	3255	3265	3277	rBV5	5739	11132	2.46%	0.288%
23	11.622	3277	3291	3305	rBV	152841	246397	54.53%	6.372%
24	15.924	4620	4629	4632	rBV9	4561	7776	1.72%	0.201%
25	16.178	4703	4708	4715	rVB7	6019	6899	1.53%	0.178%
26	16.307	4739	4748	4758	rVB2	16364	23778	5.26%	0.615%




Sum of corrected areas: 3867119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027637.D
Acq On : 01 Sep 2022 00:18
Operator : SY/MD
Sample : N4366-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

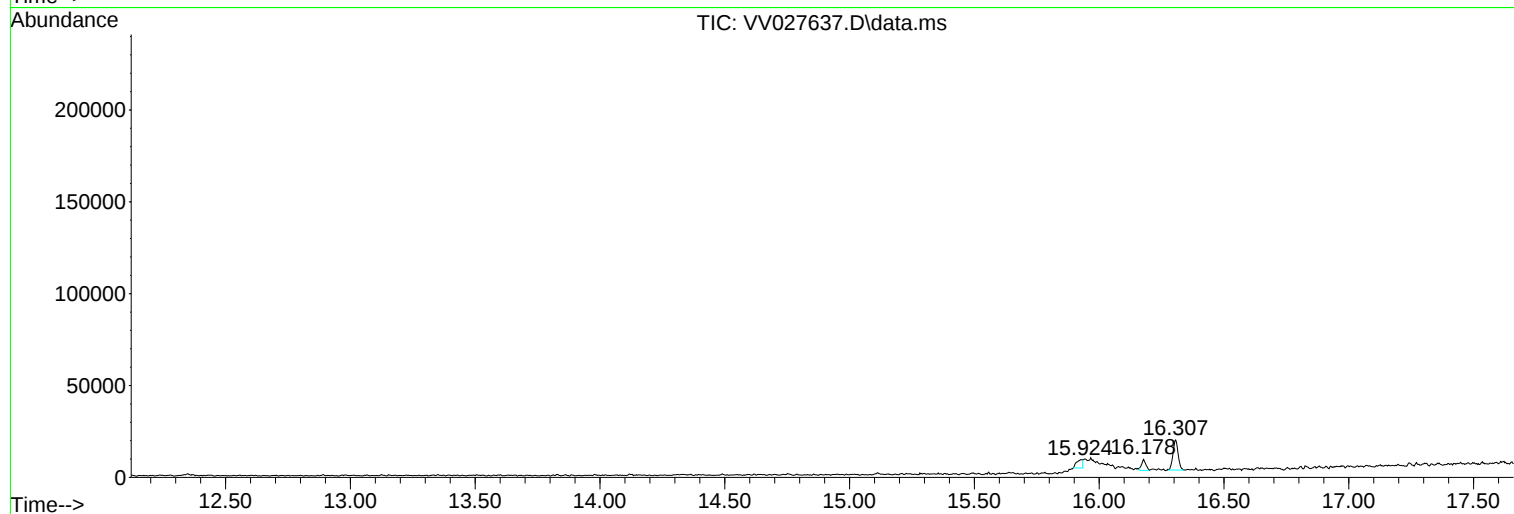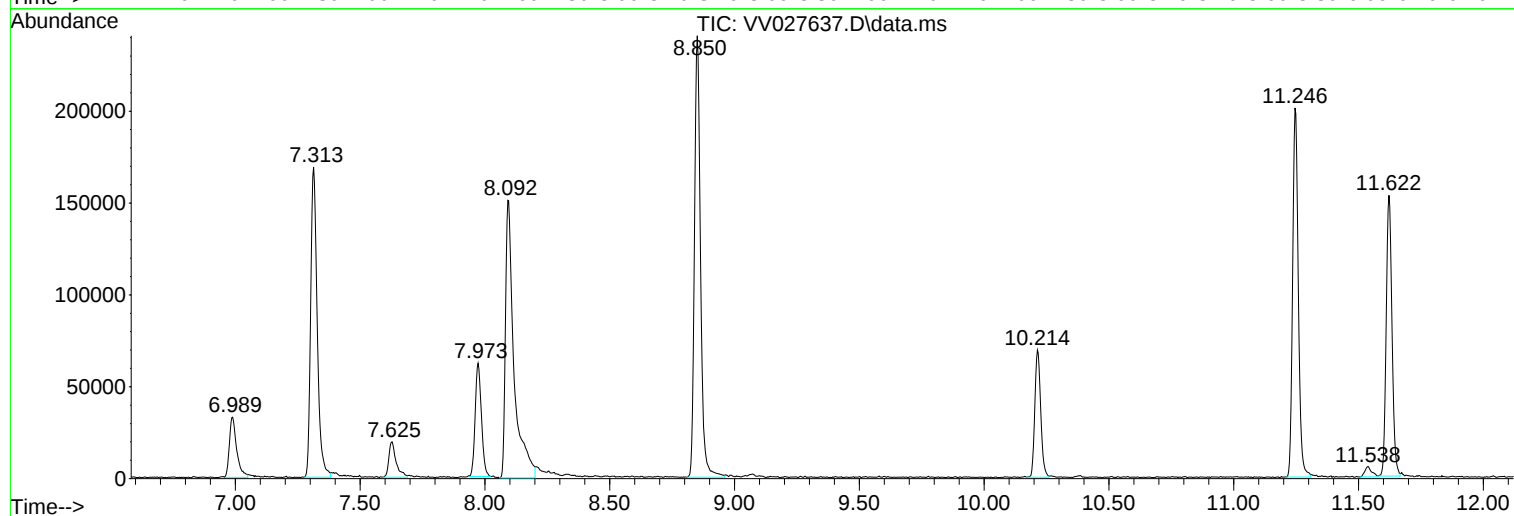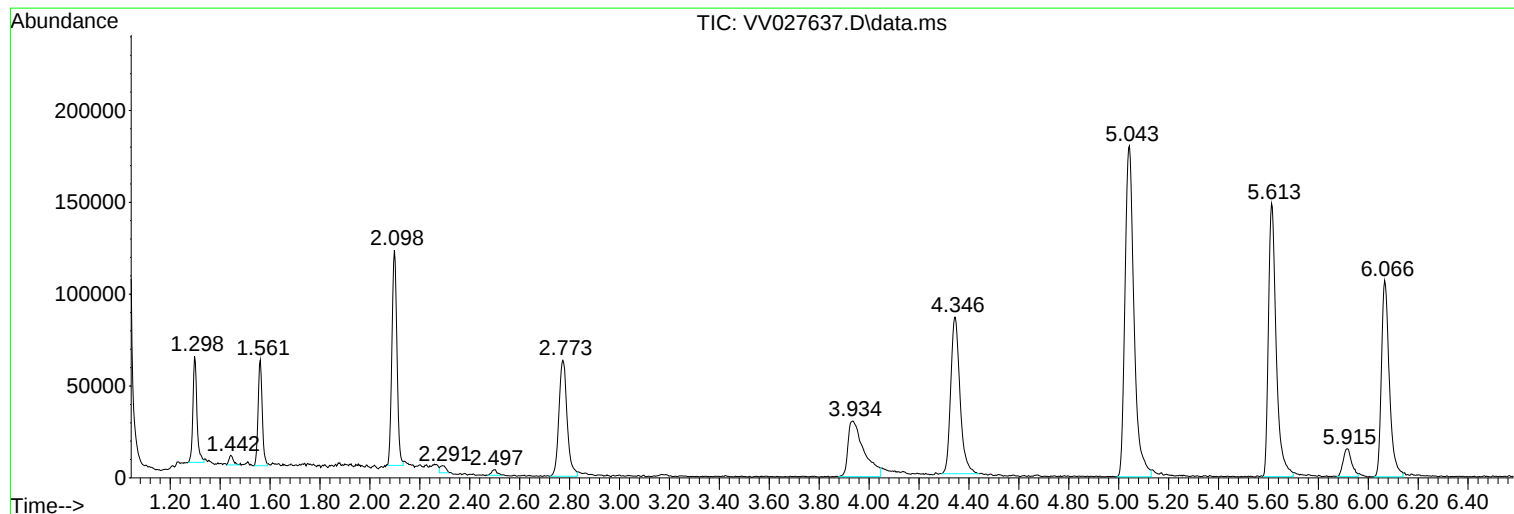

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027637.D
Acq On : 01 Sep 2022 00:18
Operator : SY/MD
Sample : N4366-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027637.D
Acq On : 01 Sep 2022 00:18
Operator : SY/MD
Sample : N4366-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc