

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027643.D
 Acq On : 01 Sep 2022 02:45
 Operator : SY/MD
 Sample : N4370-08DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E89DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	72	80	97	rBV	98582	109632	16.30%	2.056%
2	1.558	154	161	171	rBV	90869	101972	15.16%	1.912%
3	2.098	317	329	340	rBV	194157	272818	40.56%	5.116%
4	2.497	445	453	462	rVB	19047	27676	4.11%	0.519%
5	2.773	526	539	556	rBV	160191	340917	50.69%	6.393%
6	3.963	884	909	930	rBV2	64365	269551	40.08%	5.055%
7	4.352	1015	1030	1052	rBV	128831	310250	46.13%	5.818%
8	5.034	1229	1242	1260	rBV2	318617	672585	100.00%	12.612%
9	5.596	1407	1417	1440	rVB	188078	389322	57.88%	7.300%
10	6.063	1547	1562	1584	rVB	172475	362960	53.96%	6.806%
11	6.629	1724	1738	1754	rVB3	4002	11972	1.78%	0.224%
12	6.944	1830	1836	1842	rBV4	5055	8465	1.26%	0.159%
13	6.998	1843	1853	1874	rVB	73704	135918	20.21%	2.549%
14	7.323	1942	1954	1974	rBV	302142	524029	77.91%	9.826%
15	7.635	2040	2051	2069	rBV	38752	71237	10.59%	1.336%
16	8.117	2189	2201	2239	rBV2	236099	522745	77.72%	9.802%
17	8.857	2419	2431	2452	rBV	233457	379356	56.40%	7.114%
18	10.220	2842	2855	2877	rBV	100674	158936	23.63%	2.980%
19	11.249	3164	3175	3198	rBV	194830	302645	45.00%	5.675%
20	11.622	3281	3291	3310	rBV	225281	359898	53.51%	6.749%




Sum of corrected areas: 5332884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027643.D
Acq On : 01 Sep 2022 02:45
Operator : SY/MD
Sample : N4370-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

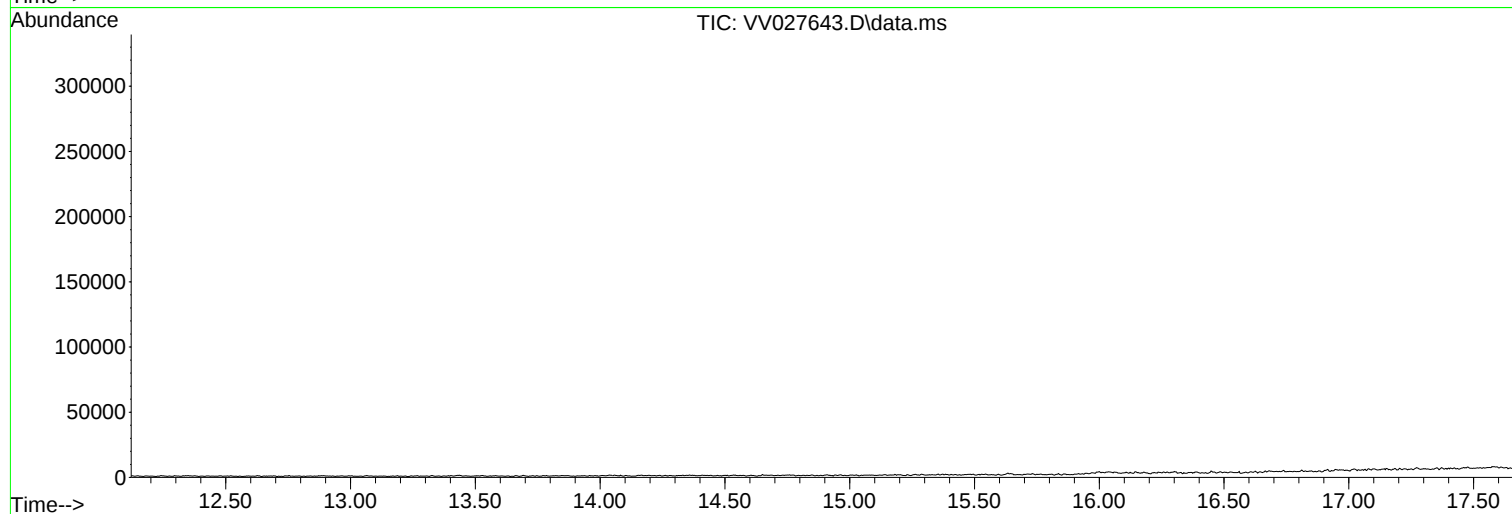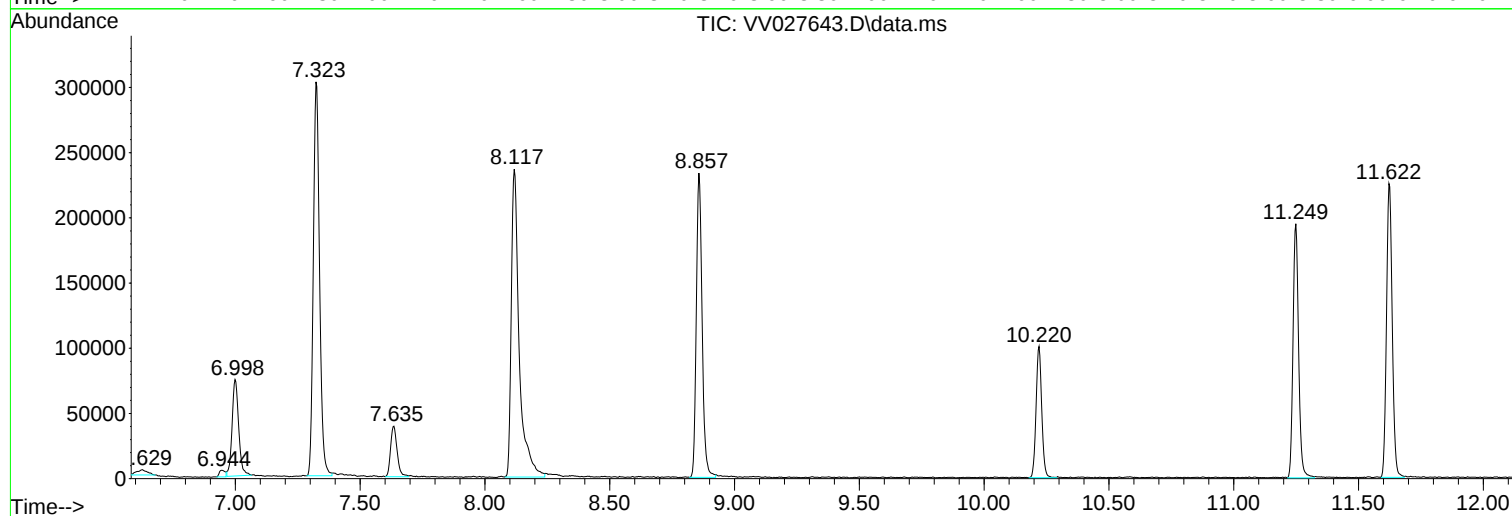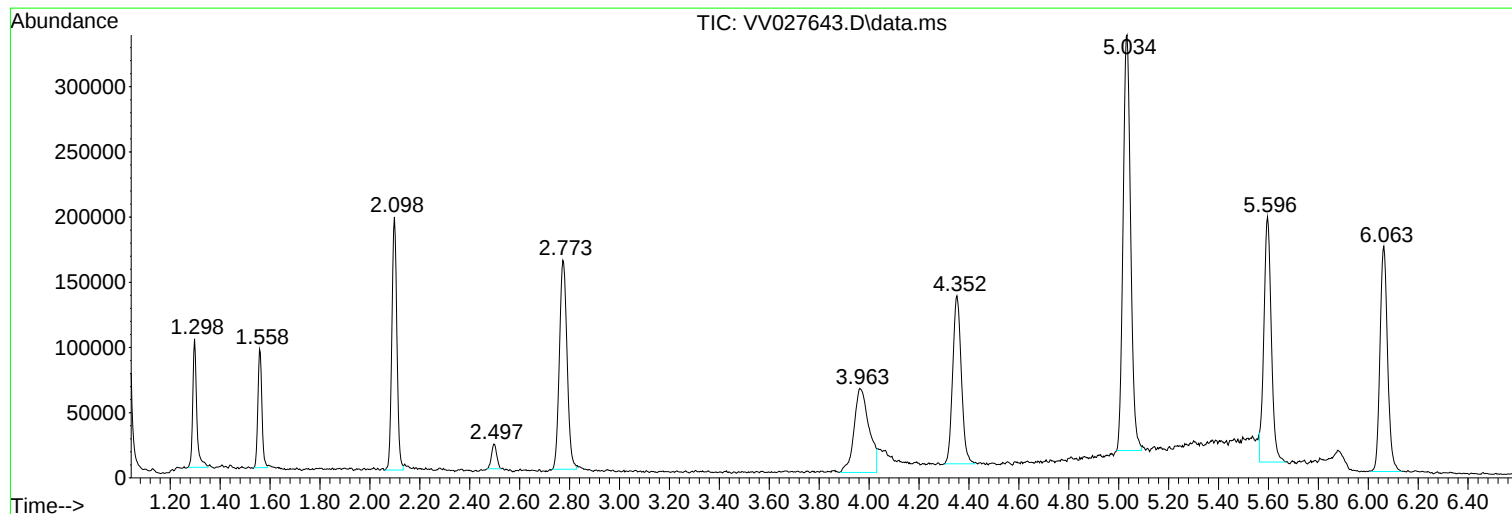

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027643.D
Acq On : 01 Sep 2022 02:45
Operator : SY/MD
Sample : N4370-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027643.D
Acq On : 01 Sep 2022 02:45
Operator : SY/MD
Sample : N4370-08DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc