

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027644.D
 Acq On : 01 Sep 2022 03:09
 Operator : SY/MD
 Sample : N4370-09DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E90DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	73	81	99	rBV	96406	110618	15.79%	2.194%
2	1.581	160	168	181	rBV	89595	112938	16.12%	2.240%
3	2.137	330	341	355	rBV	197791	285272	40.71%	5.659%
4	2.532	457	464	474	rVB2	20856	28982	4.14%	0.575%
5	2.806	536	549	568	rBV	149729	315759	45.06%	6.263%
6	3.992	901	918	919	rBV	43780	82424	11.76%	1.635%
7	4.378	1022	1038	1055	rBV	132548	315854	45.07%	6.265%
8	5.056	1234	1249	1266	rBV2	326110	700749	100.00%	13.900%
9	5.632	1414	1428	1448	rBV	166492	341466	48.73%	6.773%
10	5.912	1499	1515	1516	rBV6	6463	10179	1.45%	0.202%
11	6.092	1554	1571	1591	rBV	172984	353081	50.39%	7.004%
12	6.551	1706	1714	1723	rBV3	4823	11904	1.70%	0.236%
13	7.014	1848	1858	1882	rBV	62957	115137	16.43%	2.284%
14	7.339	1945	1959	1983	rBV	286658	505372	72.12%	10.024%
15	7.645	2046	2054	2068	rBV	35892	63167	9.01%	1.253%
16	8.120	2190	2202	2234	rBV2	225074	496544	70.86%	9.849%
17	8.863	2422	2433	2453	rBV	233938	377770	53.91%	7.493%
18	10.220	2842	2855	2872	rBV	99664	157530	22.48%	3.125%
19	11.249	3165	3175	3192	rBV	188202	293191	41.84%	5.816%
20	11.625	3277	3292	3312	rBV	225413	363438	51.86%	7.209%




Sum of corrected areas: 5041375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027644.D
Acq On : 01 Sep 2022 03:09
Operator : SY/MD
Sample : N4370-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

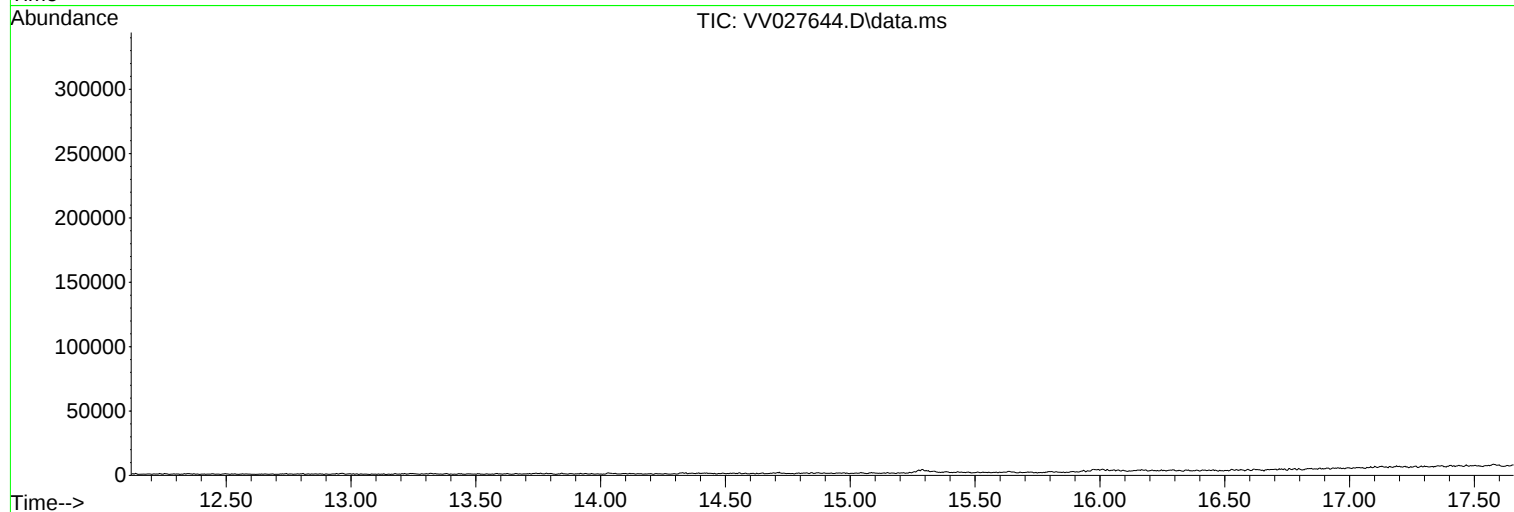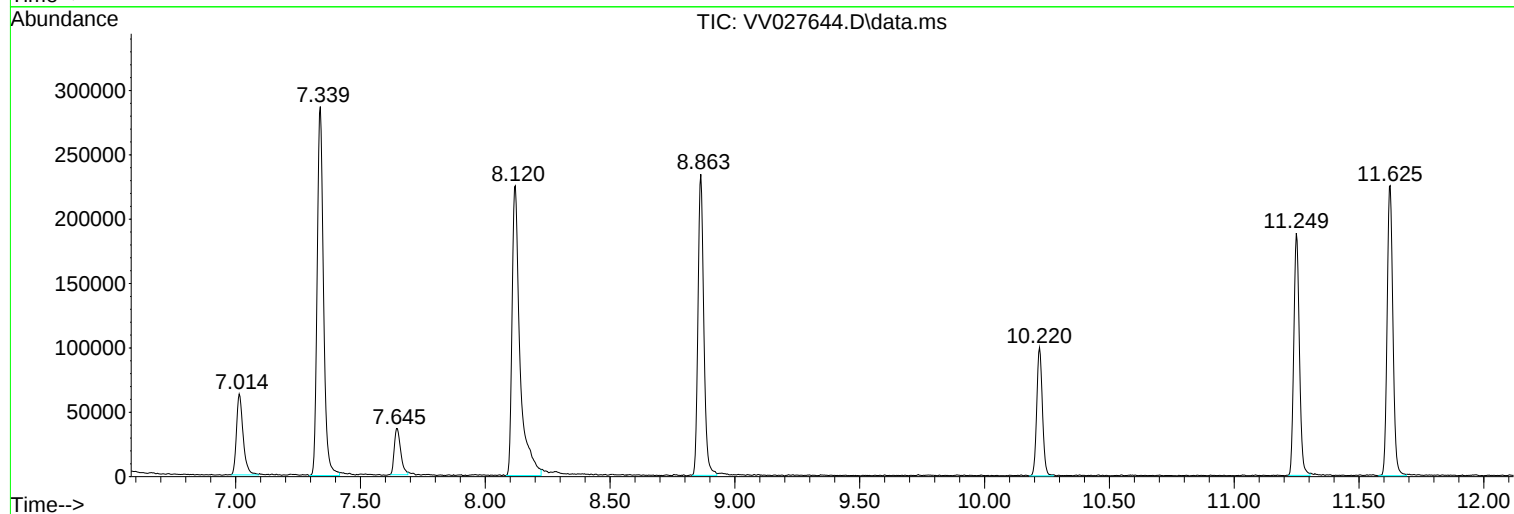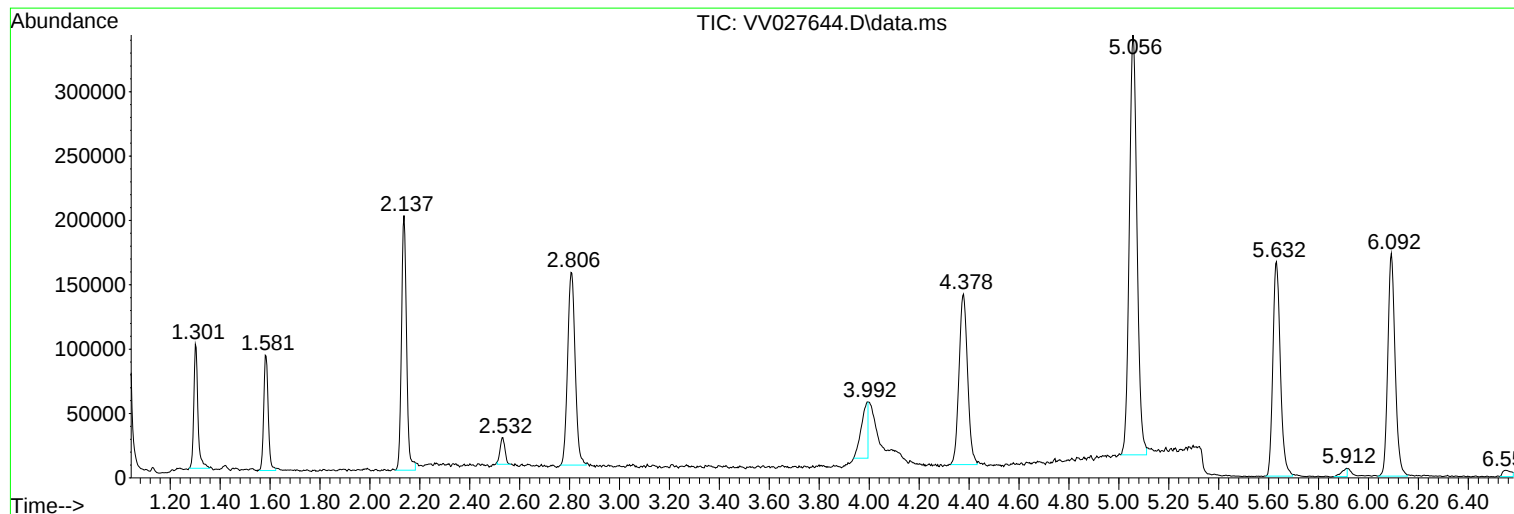

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027644.D
Acq On : 01 Sep 2022 03:09
Operator : SY/MD
Sample : N4370-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027644.D
Acq On : 01 Sep 2022 03:09
Operator : SY/MD
Sample : N4370-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc