

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027645.D
 Acq On : 01 Sep 2022 03:34
 Operator : SY/MD
 Sample : N4370-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	72	80	89	rBV	100977	104811	15.88%	2.197%
2	1.558	154	161	172	rBV	90489	101368	15.36%	2.125%
3	2.098	317	329	341	rBV	191114	272814	41.34%	5.718%
4	2.773	524	539	551	rBV4	18602	44592	6.76%	0.935%
5	4.355	1015	1031	1050	rBV	128907	305474	46.28%	6.402%
6	5.034	1229	1242	1259	rBV2	312388	659985	100.00%	13.833%
7	5.590	1404	1415	1430	rBV	175894	324761	49.21%	6.807%
8	5.879	1489	1505	1523	rBV	146390	291085	44.10%	6.101%
9	6.050	1543	1558	1581	rBV	169488	352733	53.45%	7.393%
10	7.008	1842	1856	1876	rBV2	60445	111640	16.92%	2.340%
11	7.333	1945	1957	1976	rBV	275974	481789	73.00%	10.098%
12	7.641	2042	2053	2066	rBV	36229	62118	9.41%	1.302%
13	7.989	2152	2161	2172	rVB4	6694	11229	1.70%	0.235%
14	8.117	2191	2201	2236	rBV2	216464	481824	73.01%	10.098%
15	8.860	2421	2432	2451	rBV	213622	358225	54.28%	7.508%
16	10.220	2843	2855	2871	rBV	96191	153989	23.33%	3.227%
17	11.249	3164	3175	3195	rBV	187184	283783	43.00%	5.948%
18	11.625	3280	3292	3313	rBV	215115	343202	52.00%	7.193%
19	15.895	4610	4620	4622	rBV8	10304	14376	2.18%	0.301%
20	16.705	4865	4872	4882	rVB4	8815	11452	1.74%	0.240%




Sum of corrected areas: 4771250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027645.D
Acq On : 01 Sep 2022 03:34
Operator : SY/MD
Sample : N4370-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

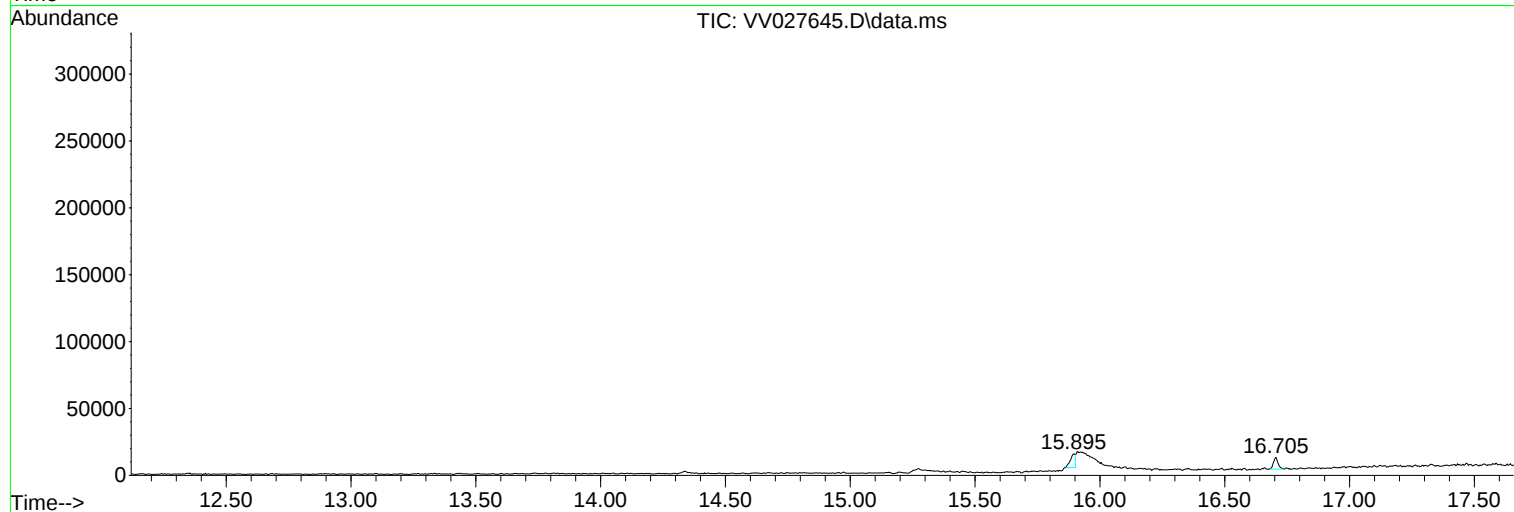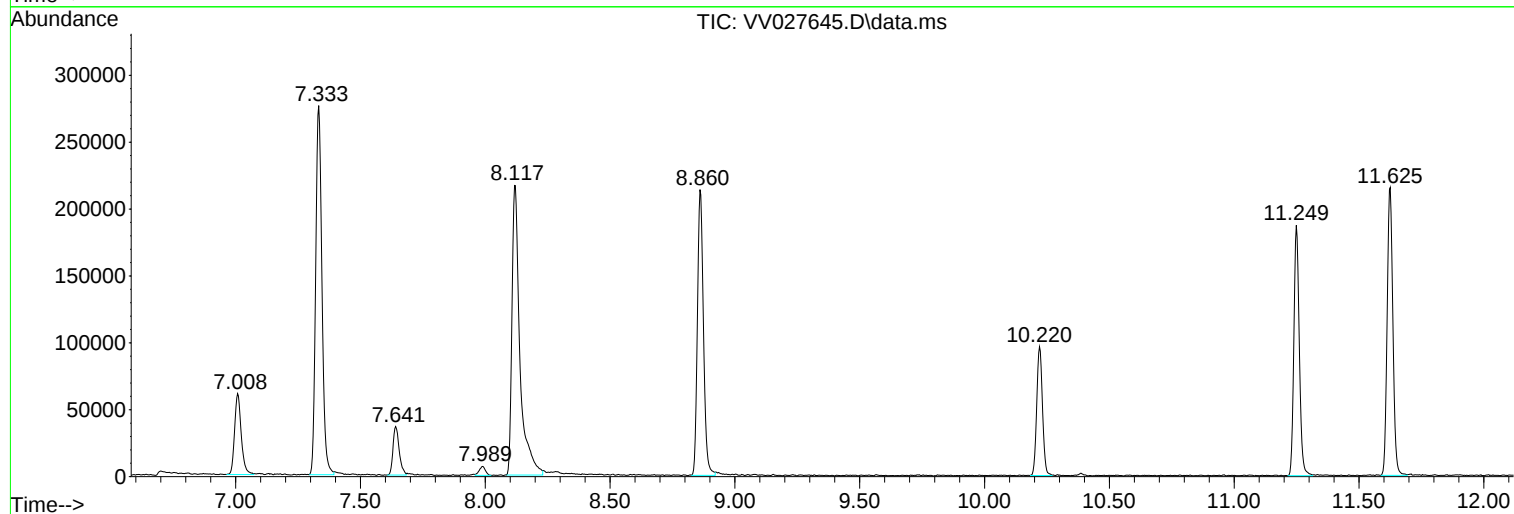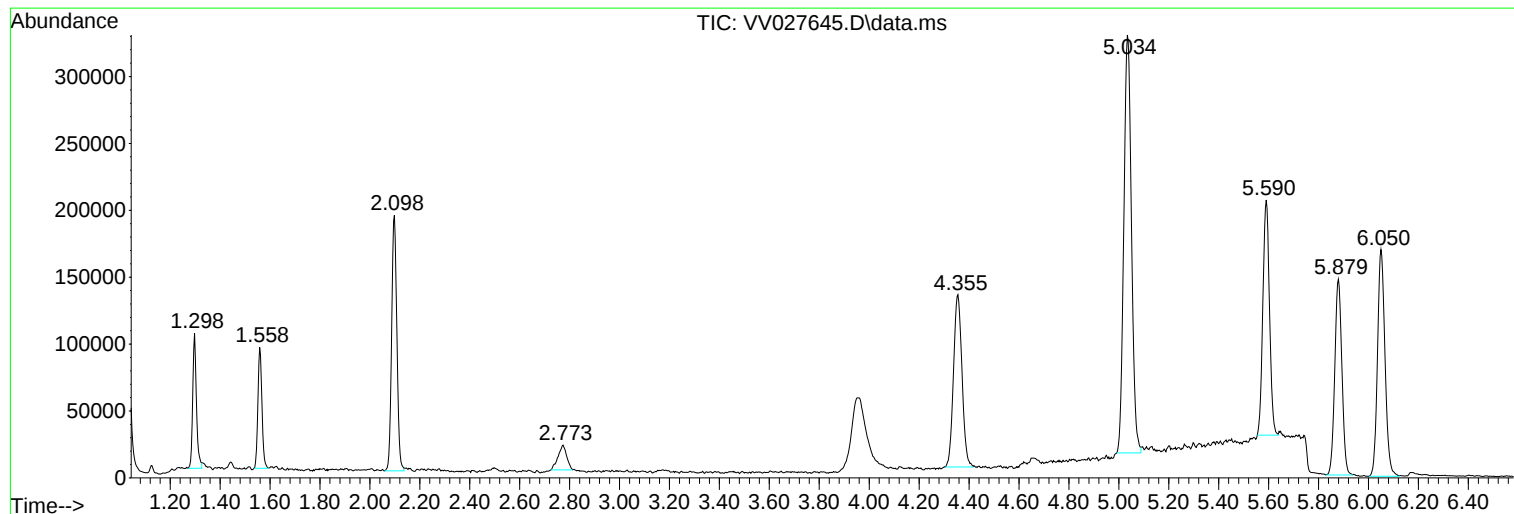

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027645.D
Acq On : 01 Sep 2022 03:34
Operator : SY/MD
Sample : N4370-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027645.D
Acq On : 01 Sep 2022 03:34
Operator : SY/MD
Sample : N4370-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc