

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027648.D
 Acq On : 01 Sep 2022 04:47
 Operator : SY/MD
 Sample : N4400-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rBV	98841	106127	15.98%	2.093%
2	1.568	156	164	177	rBV	96095	112641	16.96%	2.221%
3	2.108	321	332	345	rBV	198214	284545	42.85%	5.611%
4	3.892	875	887	911	rBV2	33602	122286	18.41%	2.411%
5	4.349	1012	1029	1061	rBV3	142718	463208	69.75%	9.134%
6	5.047	1227	1246	1270	rBV2	260384	664102	100.00%	13.095%
7	5.616	1409	1423	1454	rBV	144636	308389	46.44%	6.081%
8	5.915	1502	1516	1527	rBV	6250	15190	2.29%	0.300%
9	6.066	1549	1563	1590	rBV2	155323	331535	49.92%	6.537%
10	6.513	1690	1702	1712	rBV4	4403	9155	1.38%	0.181%
11	6.985	1836	1849	1872	rBV	55619	111609	16.81%	2.201%
12	7.313	1940	1951	1971	rBV	269198	488618	73.58%	9.635%
13	7.622	2037	2047	2066	rBV	33186	64436	9.70%	1.271%
14	7.972	2142	2156	2175	rBV	153752	263876	39.73%	5.203%
15	8.091	2182	2193	2227	rBV2	174103	490585	73.87%	9.674%
16	8.850	2418	2429	2450	rBV	230276	390620	58.82%	7.702%
17	10.214	2842	2853	2867	rBV	92854	153218	23.07%	3.021%
18	11.249	3164	3175	3194	rBV	193497	310995	46.83%	6.132%
19	11.535	3254	3264	3275	rBV5	6447	12226	1.84%	0.241%
20	11.622	3279	3291	3313	rVV	226360	368048	55.42%	7.257%




Sum of corrected areas: 5071409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027648.D
Acq On : 01 Sep 2022 04:47
Operator : SY/MD
Sample : N4400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

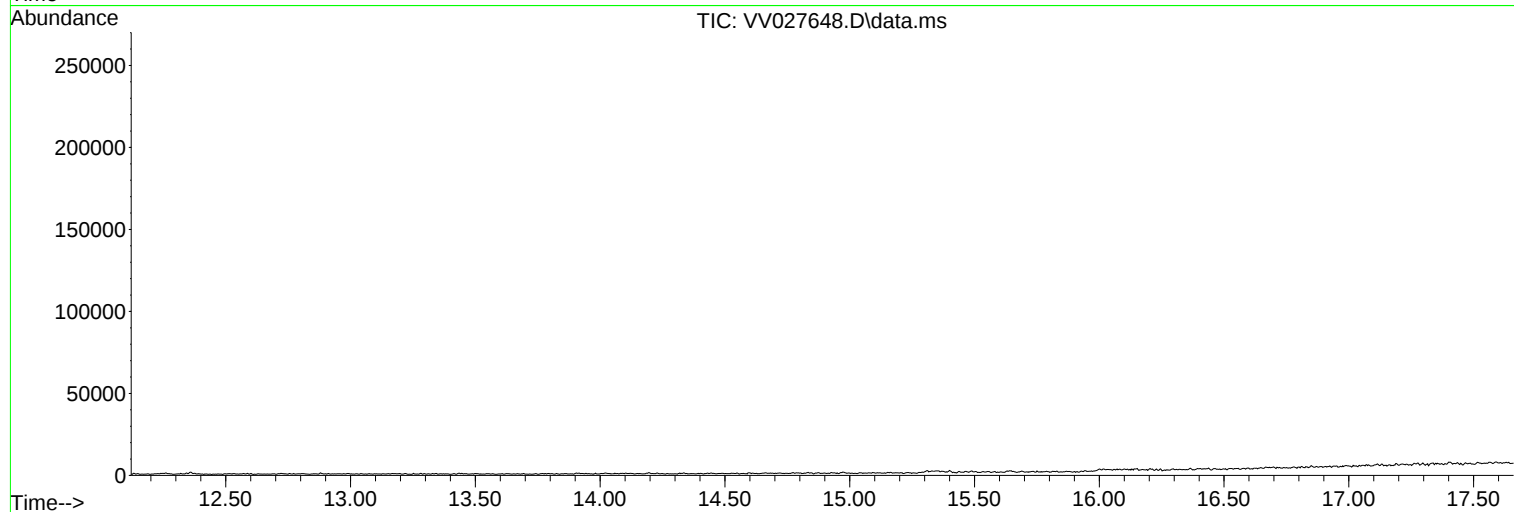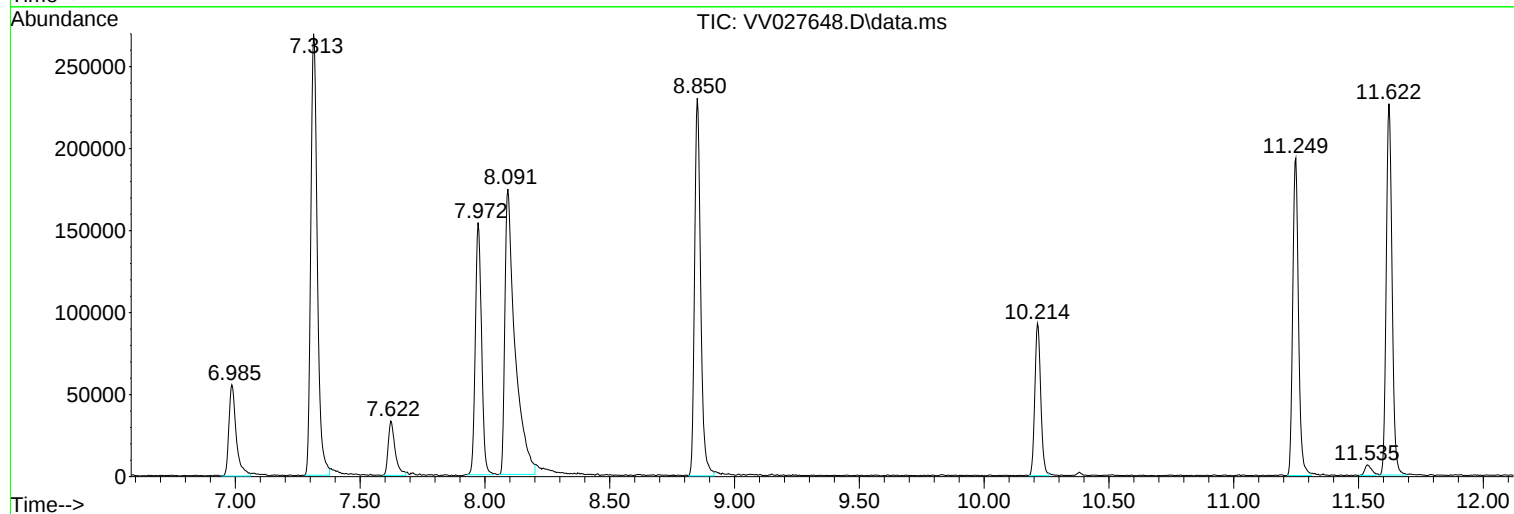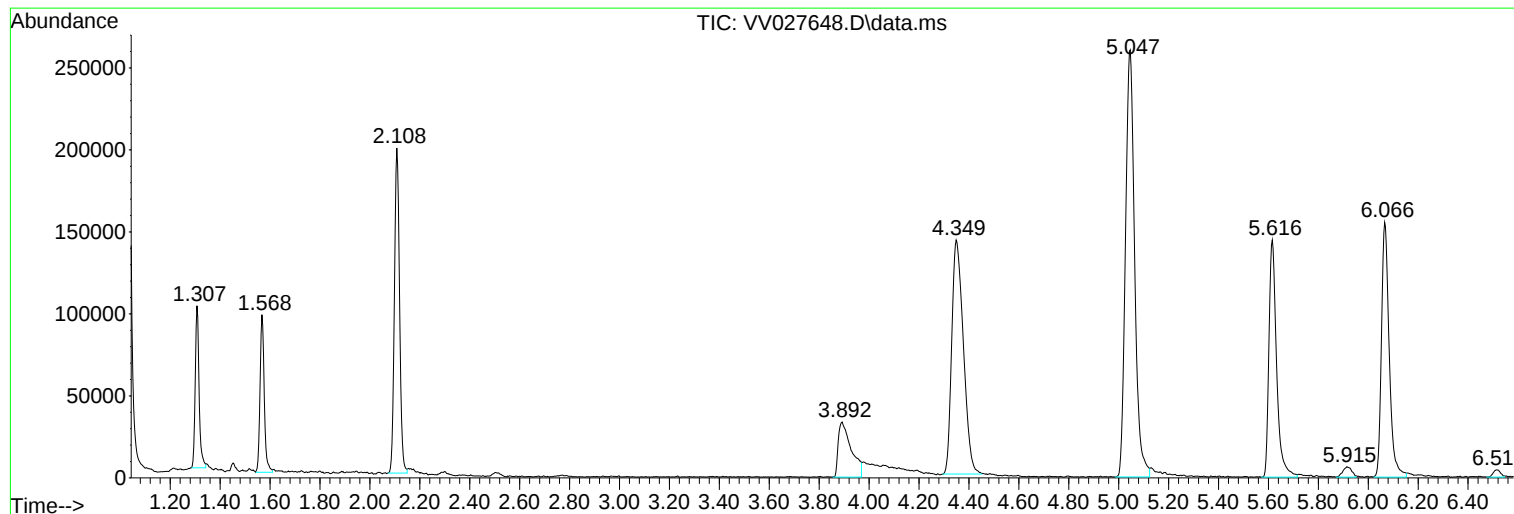

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027648.D
Acq On : 01 Sep 2022 04:47
Operator : SY/MD
Sample : N4400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027648.D
Acq On : 01 Sep 2022 04:47
Operator : SY/MD
Sample : N4400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc