

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027649.D
 Acq On : 01 Sep 2022 05:11
 Operator : SY/MD
 Sample : N4400-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	38	rVB2	14322	16813	2.48%	0.343%
2	1.307	73	83	103	rBV	102003	120236	17.75%	2.456%
3	1.568	156	164	174	rBV	95339	110710	16.35%	2.261%
4	2.108	321	332	348	rBV	195789	285045	42.09%	5.822%
5	2.770	527	538	548	rBV4	3398	7516	1.11%	0.154%
6	3.899	877	889	916	rBV3	41696	163802	24.19%	3.346%
7	4.346	1011	1028	1052	rBV	125696	317069	46.82%	6.476%
8	5.043	1226	1245	1275	rBV3	264343	677253	100.00%	13.832%
9	5.616	1411	1423	1452	rBV2	151067	322309	47.59%	6.583%
10	5.915	1503	1516	1522	rBV7	6072	12786	1.89%	0.261%
11	6.066	1550	1563	1591	rBV	157733	335018	49.47%	6.842%
12	6.985	1837	1849	1870	rBV2	55682	113139	16.71%	2.311%
13	7.313	1939	1951	1971	rBV	280185	502448	74.19%	10.262%
14	7.622	2037	2047	2068	rBV2	33063	64621	9.54%	1.320%
15	8.091	2182	2193	2227	rBV2	187040	506615	74.80%	10.347%
16	8.850	2418	2429	2452	rBV	239142	398533	58.85%	8.140%
17	10.214	2841	2853	2870	rBV	96051	154872	22.87%	3.163%
18	11.246	3160	3174	3193	rBV	200899	325565	48.07%	6.649%
19	11.532	3253	3263	3280	rBV	30632	57305	8.46%	1.170%
20	11.622	3280	3291	3306	rVV	240437	385484	56.92%	7.873%
21	15.924	4613	4629	4630	rBV	9856	19029	2.81%	0.389%




Sum of corrected areas: 4896168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027649.D
Acq On : 01 Sep 2022 05:11
Operator : SY/MD
Sample : N4400-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

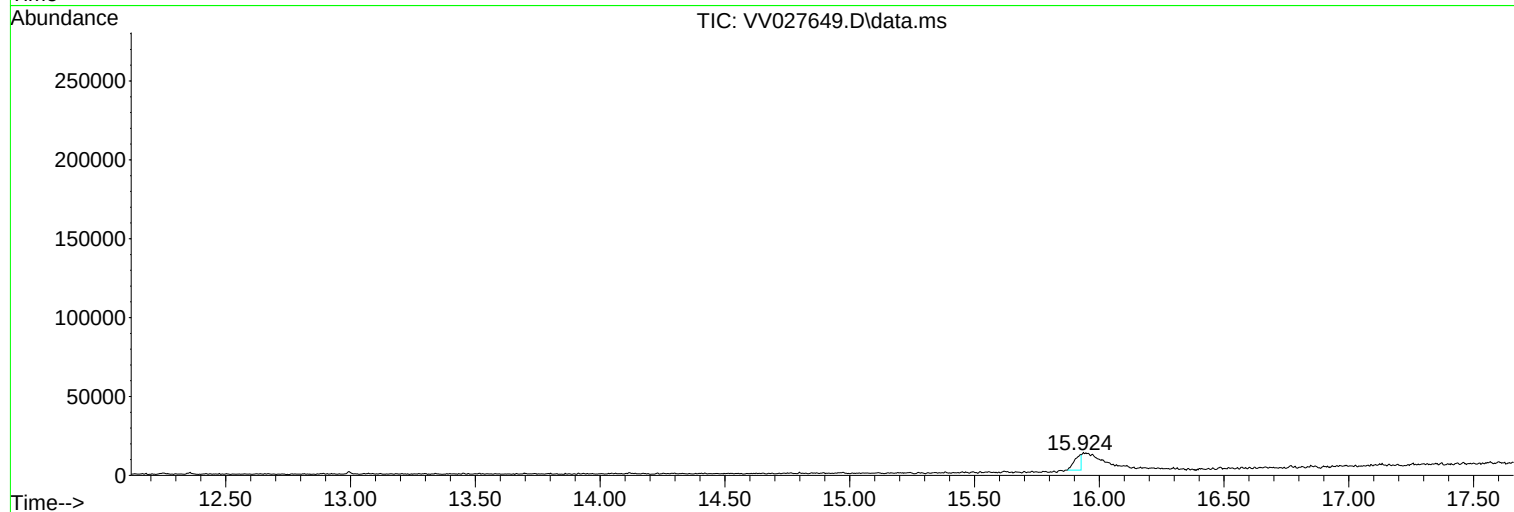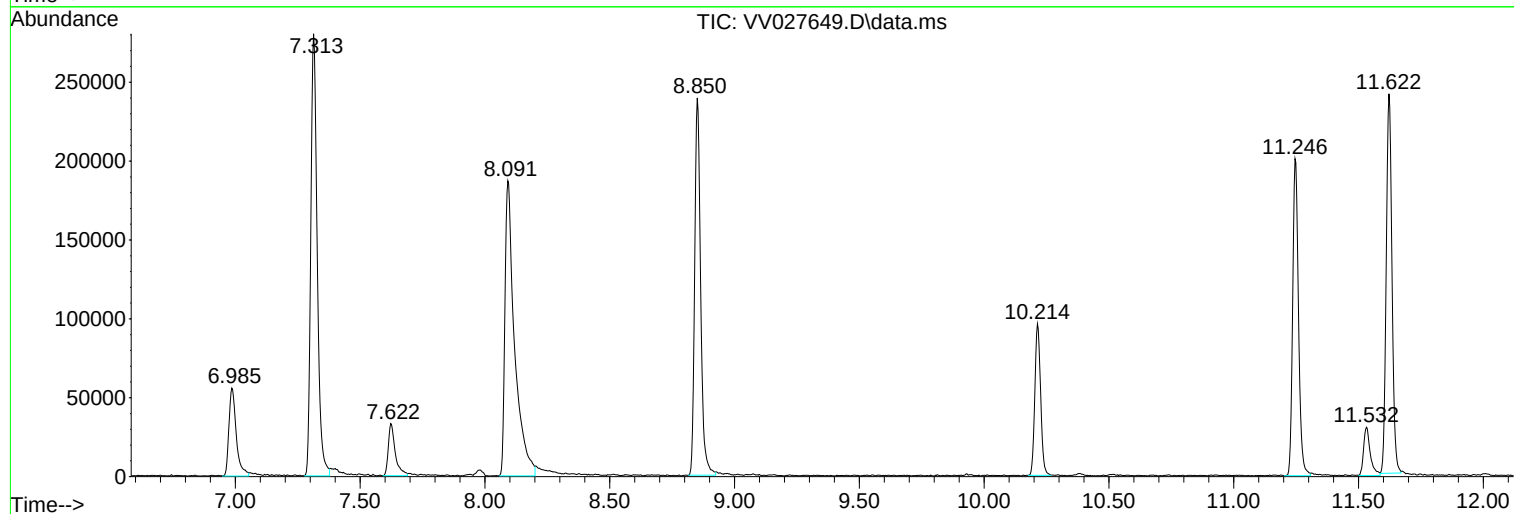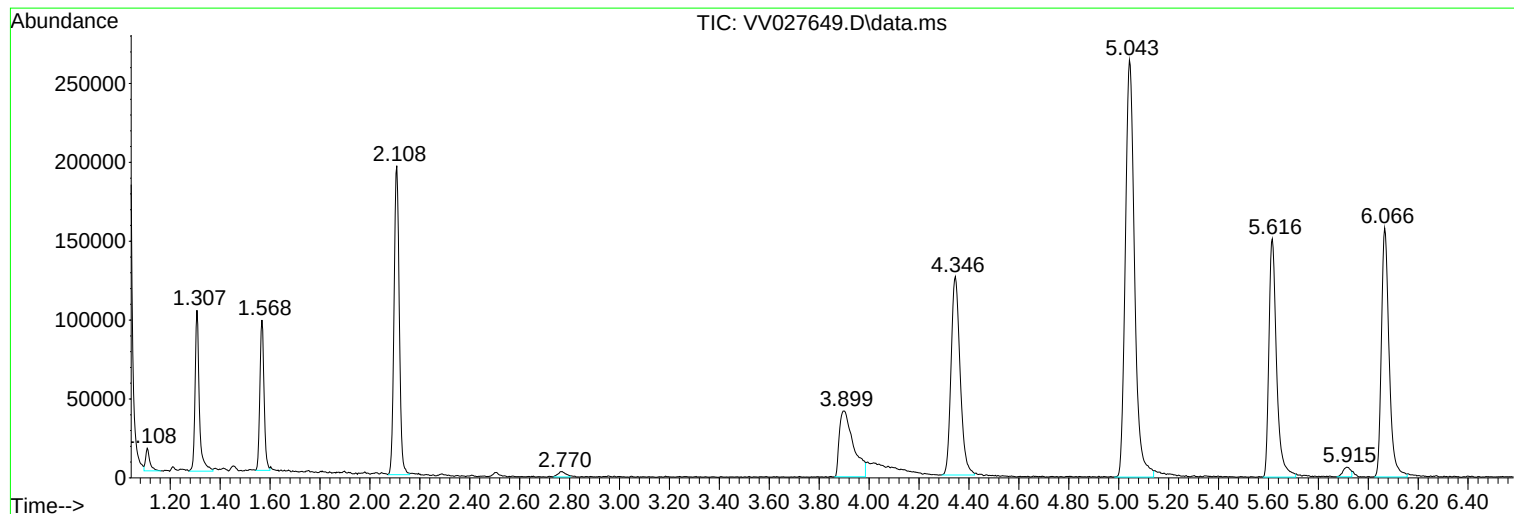

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027649.D
Acq On : 01 Sep 2022 05:11
Operator : SY/MD
Sample : N4400-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.532	0.88 ug/L	57305	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83

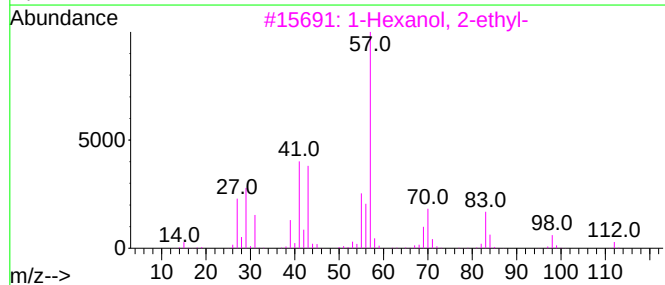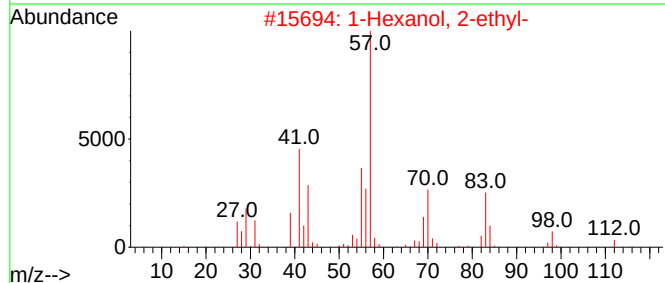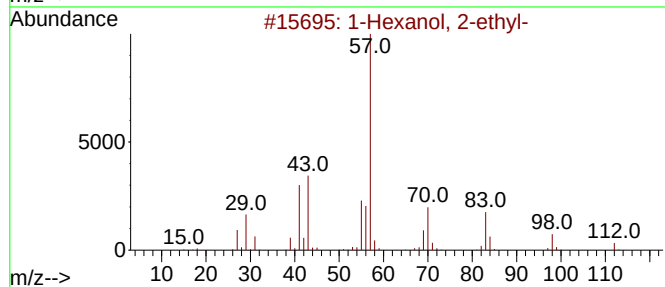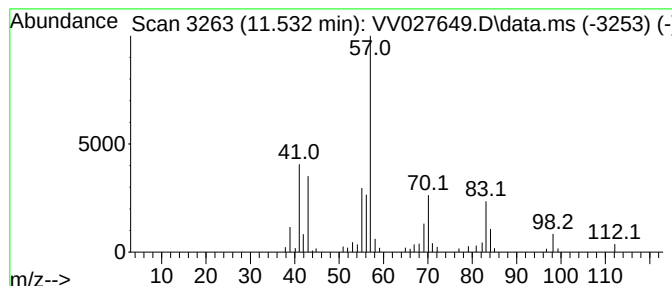

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027649.D
Acq On : 01 Sep 2022 05:11
Operator : SY/MD
Sample : N4400-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.532	0.9	ug/L	57305	3	11.249	325565	5.0