

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027652.D
 Acq On : 01 Sep 2022 06:24
 Operator : SY/MD
 Sample : N4400-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	100	rBV	100426	116348	16.71%	2.351%
2	1.452	123	128	133	rBV4	6861	7624	1.09%	0.154%
3	1.568	157	164	176	rBV	96735	110512	15.87%	2.233%
4	2.108	322	332	349	rVB	202747	289836	41.62%	5.856%
5	2.770	526	538	551	rBV3	7393	16577	2.38%	0.335%
6	3.892	878	887	912	rBV2	35944	129028	18.53%	2.607%
7	4.346	1009	1028	1055	rBV	127356	322554	46.32%	6.517%
8	5.043	1230	1245	1279	rBV2	275296	696372	100.00%	14.069%
9	5.616	1411	1423	1451	rBV	151885	327535	47.03%	6.617%
10	5.918	1503	1517	1532	rVB	5934	14591	2.10%	0.295%
11	6.066	1550	1563	1586	rBV	162746	342699	49.21%	6.924%
12	6.989	1838	1850	1868	rBV	56911	114235	16.40%	2.308%
13	7.314	1940	1951	1975	rBV	288730	521702	74.92%	10.540%
14	7.625	2038	2048	2067	rBV2	32220	64637	9.28%	1.306%
15	7.976	2147	2157	2171	rVB3	27556	48833	7.01%	0.987%
16	8.092	2182	2193	2230	rBV2	193252	515235	73.99%	10.409%
17	8.850	2418	2429	2458	rBV	233874	399487	57.37%	8.071%
18	10.214	2843	2853	2871	rBV	96685	158588	22.77%	3.204%
19	11.246	3161	3174	3198	rBV	203465	330039	47.39%	6.668%
20	11.532	3254	3263	3280	rBV2	16586	31436	4.51%	0.635%
21	11.622	3280	3291	3313	rVV	240524	391818	56.27%	7.916%




Sum of corrected areas: 4949686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027652.D
Acq On : 01 Sep 2022 06:24
Operator : SY/MD
Sample : N4400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

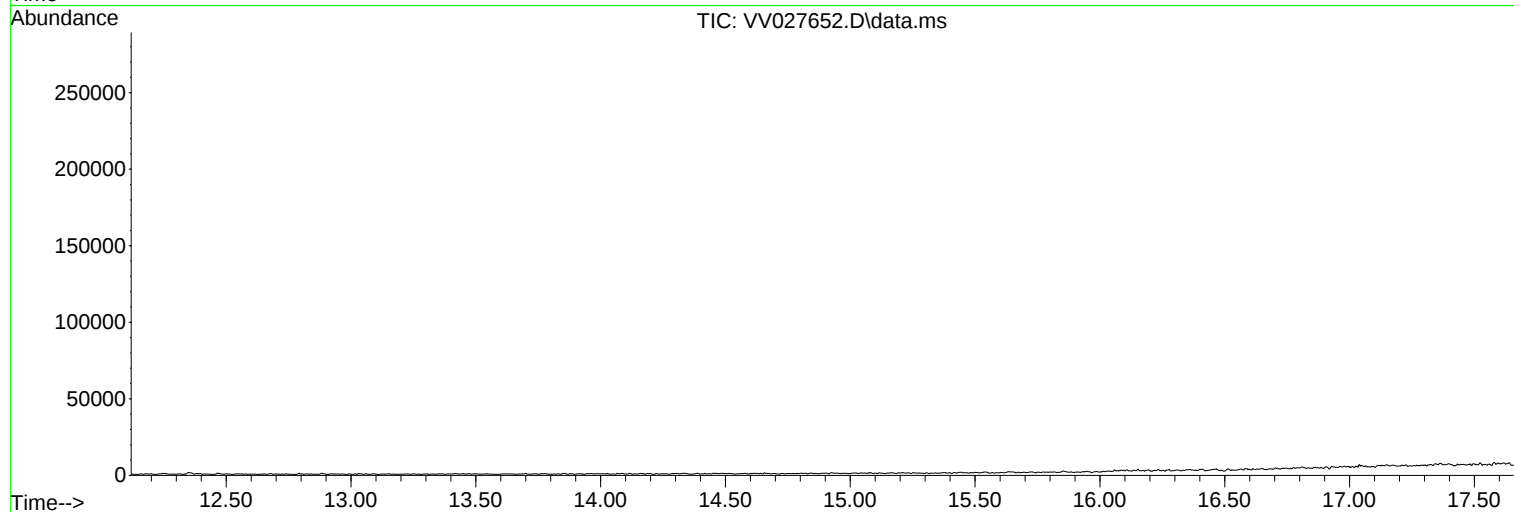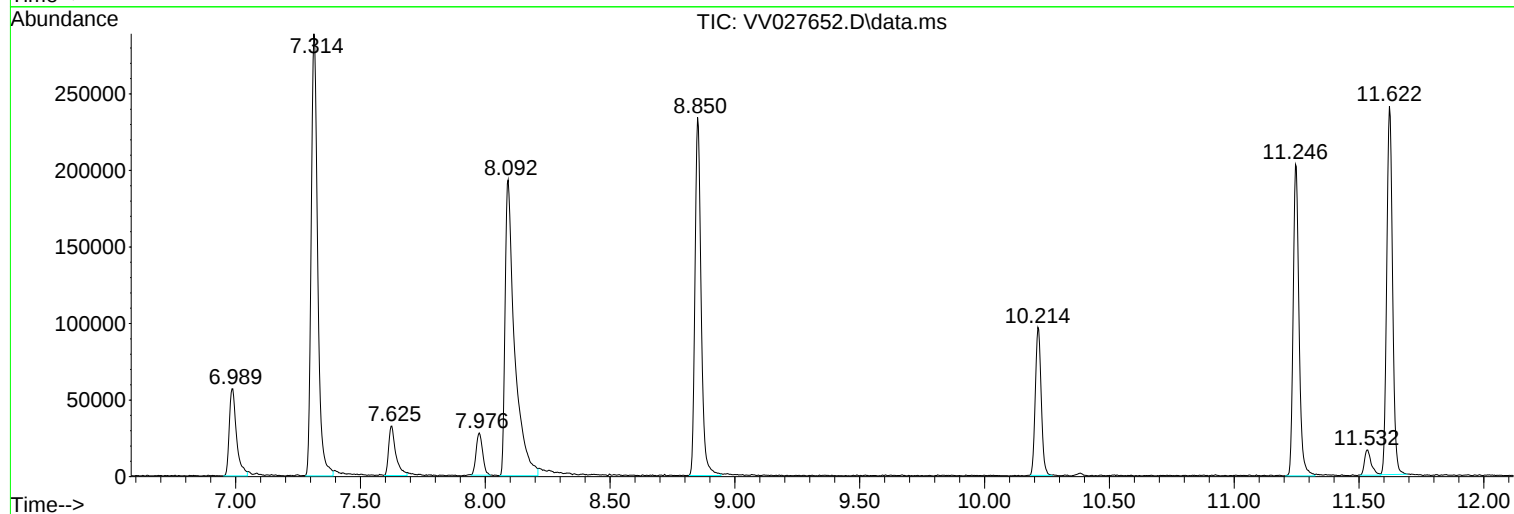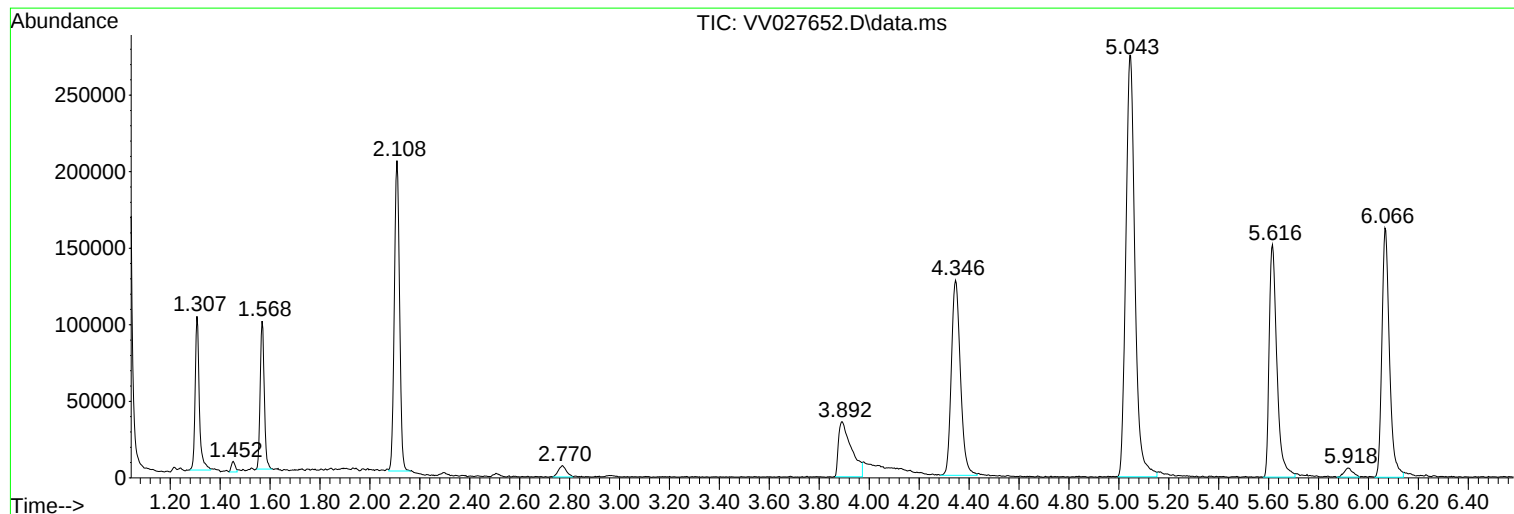

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027652.D
Acq On : 01 Sep 2022 06:24
Operator : SY/MD
Sample : N4400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027652.D
Acq On : 01 Sep 2022 06:24
Operator : SY/MD
Sample : N4400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc