

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027653.D
 Acq On : 01 Sep 2022 06:49
 Operator : SY/MD
 Sample : N4400-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rBV	98335	110008	15.87%	2.245%
2	1.568	156	164	180	rVB	96182	111567	16.10%	2.277%
3	2.108	322	332	348	rVB	196781	283994	40.98%	5.797%
4	2.767	524	537	550	rBV2	14238	30860	4.45%	0.630%
5	3.889	876	886	906	rBV	36172	116749	16.84%	2.383%
6	4.346	1011	1028	1054	rBV2	133566	366157	52.83%	7.474%
7	5.047	1229	1246	1273	rBV2	272212	693084	100.00%	14.147%
8	5.616	1411	1423	1451	rBV	151302	321519	46.39%	6.563%
9	6.066	1550	1563	1587	rBV	158325	336268	48.52%	6.864%
10	6.985	1838	1849	1869	rBV2	58478	112949	16.30%	2.306%
11	7.313	1940	1951	1979	rBV	284423	517670	74.69%	10.567%
12	7.622	2039	2047	2061	rBV	33253	60891	8.79%	1.243%
13	7.976	2148	2157	2168	rVB3	22328	37520	5.41%	0.766%
14	8.091	2182	2193	2229	rBV3	187519	508201	73.32%	10.373%
15	8.850	2418	2429	2452	rBV	234381	399535	57.65%	8.155%
16	10.214	2842	2853	2874	rBV	95883	156981	22.65%	3.204%
17	11.246	3164	3174	3195	rBV	202132	325848	47.01%	6.651%
18	11.535	3255	3264	3279	rBV5	9692	19323	2.79%	0.394%
19	11.622	3279	3291	3312	rBV	245547	389981	56.27%	7.960%




Sum of corrected areas: 4899105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027653.D
Acq On : 01 Sep 2022 06:49
Operator : SY/MD
Sample : N4400-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

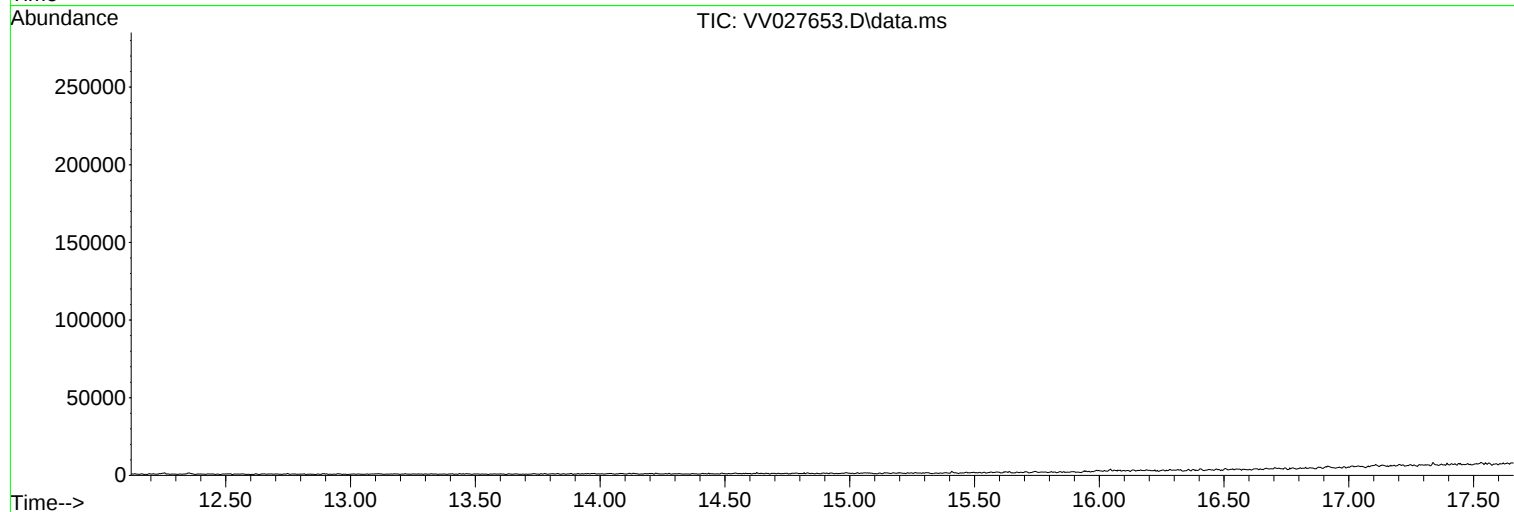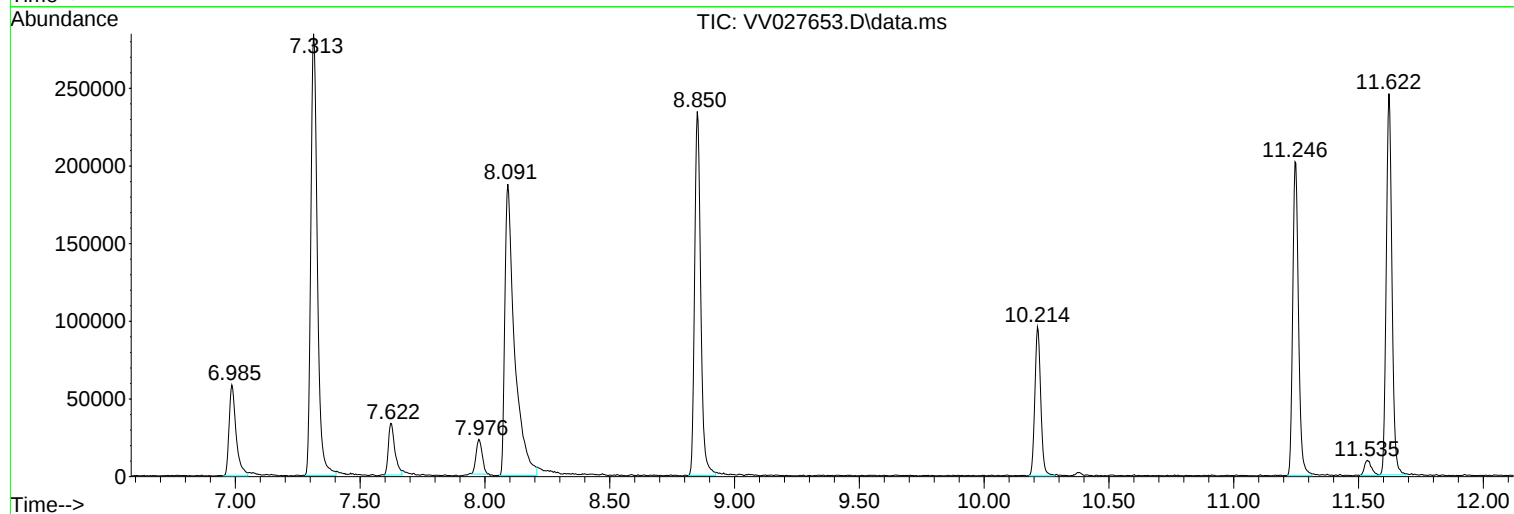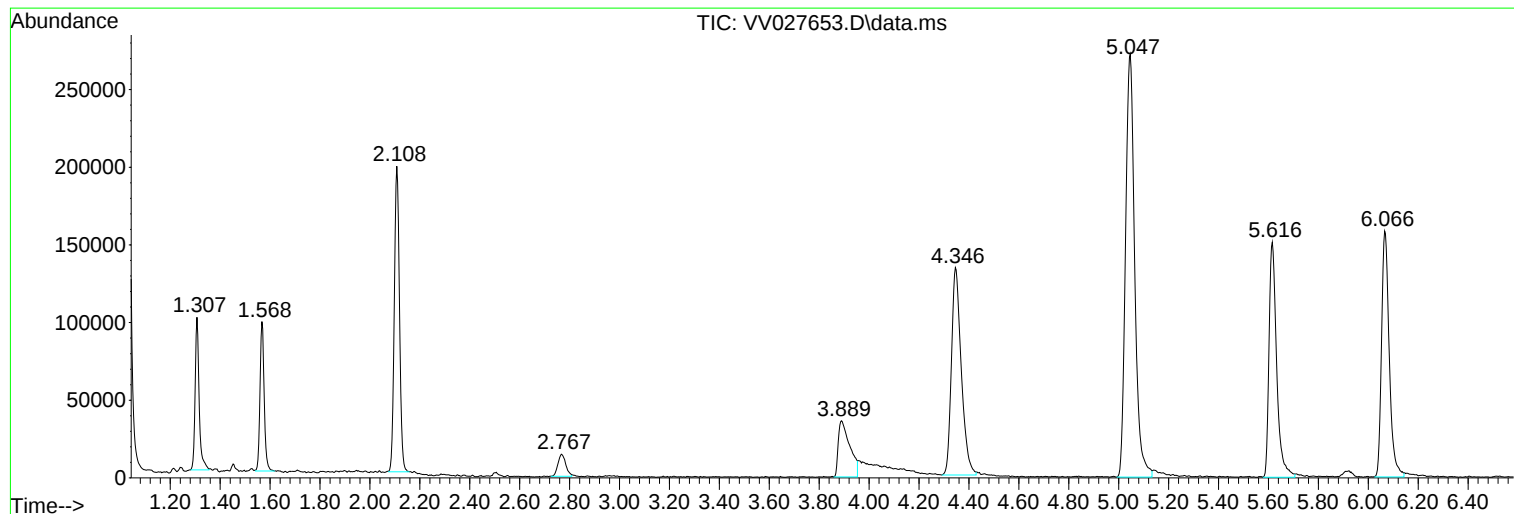

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027653.D
Acq On : 01 Sep 2022 06:49
Operator : SY/MD
Sample : N4400-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027653.D
Acq On : 01 Sep 2022 06:49
Operator : SY/MD
Sample : N4400-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc