

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027656.D
 Acq On : 01 Sep 2022 09:25
 Operator : SY/MD
 Sample : N4400-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB	104574	113960	16.55%	2.374%
2	1.568	156	164	177	rBV	97757	113048	16.41%	2.355%
3	2.108	321	332	344	rBV	197509	285937	41.52%	5.956%
4	2.764	528	536	549	rBV6	3849	7215	1.05%	0.150%
5	3.886	875	885	911	rBV2	33500	124159	18.03%	2.586%
6	4.339	1008	1026	1049	rBV2	125363	325856	47.31%	6.788%
7	5.040	1225	1244	1276	rBV2	264729	688724	100.00%	14.346%
8	5.609	1409	1421	1449	rBV	146281	313127	45.46%	6.522%
9	6.063	1549	1562	1590	rBV	157454	334984	48.64%	6.978%
10	6.982	1836	1848	1870	rBV	56402	112375	16.32%	2.341%
11	7.310	1938	1950	1975	rBV	281598	508466	73.83%	10.591%
12	7.622	2036	2047	2066	rBV	33413	65465	9.51%	1.364%
13	7.972	2147	2156	2168	rVB3	13220	23277	3.38%	0.485%
14	8.088	2180	2192	2231	rBV2	181918	501703	72.85%	10.451%
15	8.847	2416	2428	2451	rBV	227224	393661	57.16%	8.200%
16	10.214	2842	2853	2870	rBV2	93716	155129	22.52%	3.231%
17	11.246	3163	3174	3190	rBV	200412	319741	46.43%	6.660%
18	11.535	3253	3264	3279	rBV3	15785	29982	4.35%	0.625%
19	11.622	3279	3291	3309	rVV	241249	383914	55.74%	7.997%




Sum of corrected areas: 4800723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027656.D
Acq On : 01 Sep 2022 09:25
Operator : SY/MD
Sample : N4400-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

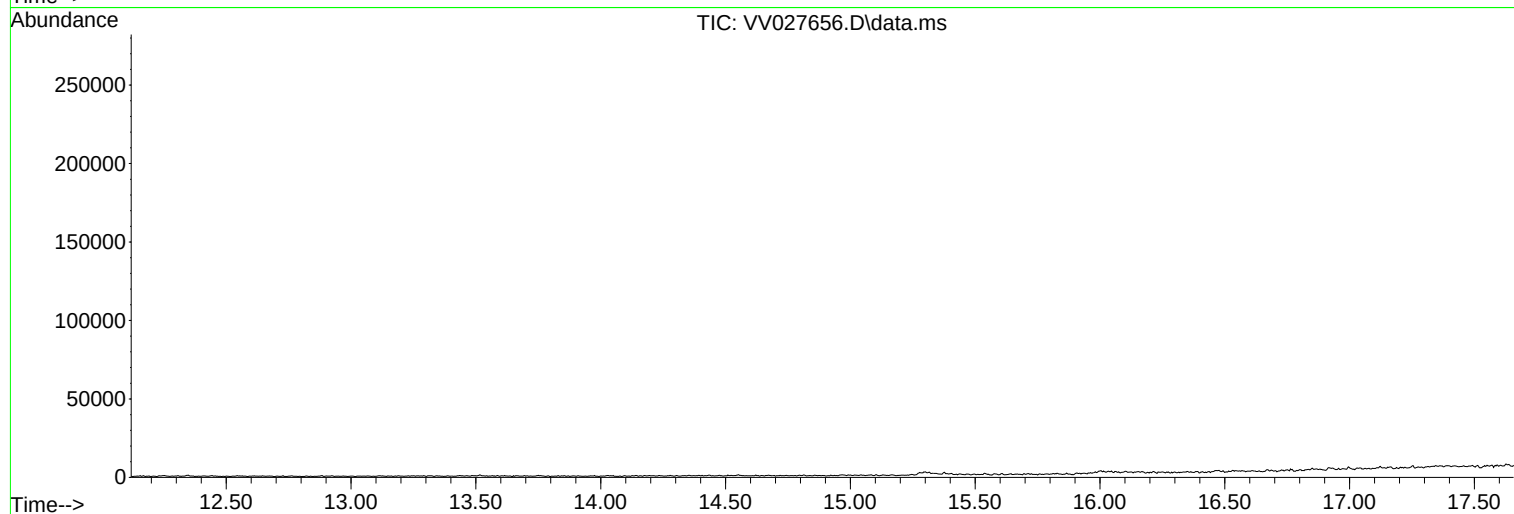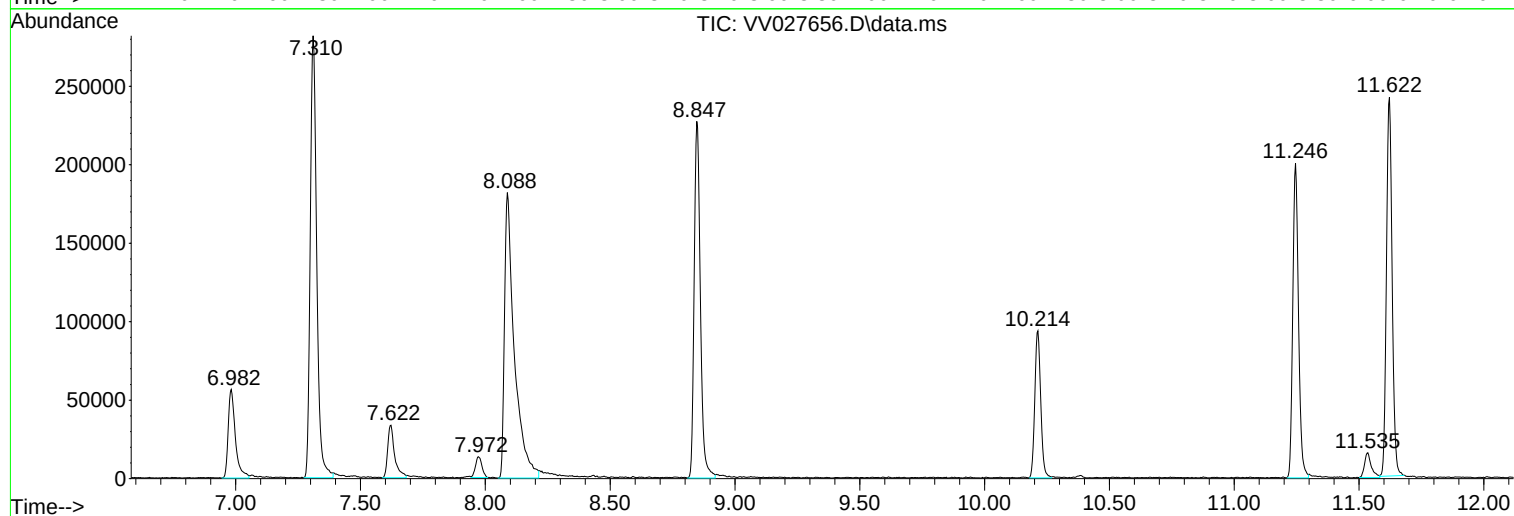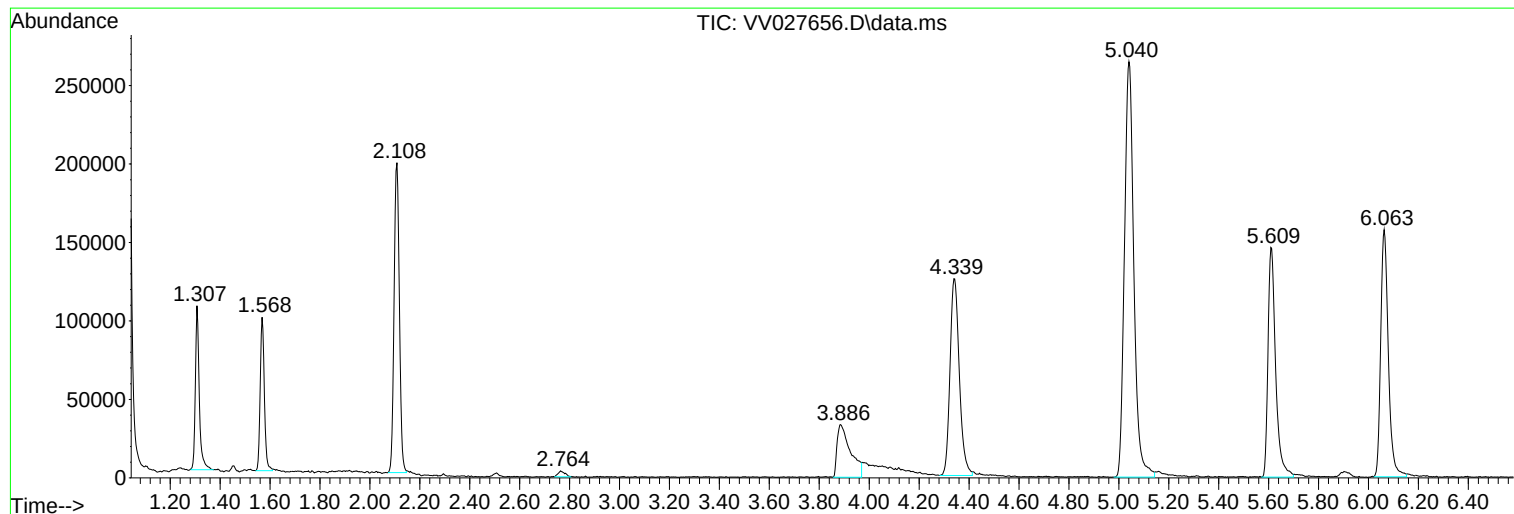

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027656.D
Acq On : 01 Sep 2022 09:25
Operator : SY/MD
Sample : N4400-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027656.D
Acq On : 01 Sep 2022 09:25
Operator : SY/MD
Sample : N4400-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc