

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027659.D
 Acq On : 01 Sep 2022 10:39
 Operator : SY/MD
 Sample : N4400-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	96	rBV	95467	110388	16.14%	2.295%
2	1.568	155	164	182	rBV	94748	111411	16.29%	2.317%
3	2.108	321	332	345	rBV	197460	282955	41.37%	5.884%
4	2.294	381	390	400	rBV	6049	9047	1.32%	0.188%
5	3.895	878	888	915	rBV2	32196	119415	17.46%	2.483%
6	4.346	1012	1028	1053	rVB	125046	306918	44.87%	6.382%
7	5.043	1227	1245	1275	rBV2	267327	683967	100.00%	14.222%
8	5.616	1411	1423	1448	rBV	147131	312657	45.71%	6.501%
9	6.066	1550	1563	1589	rBV	155624	330933	48.38%	6.881%
10	6.985	1839	1849	1866	rBV2	55906	110292	16.13%	2.293%
11	7.313	1939	1951	1971	rBV	281856	510710	74.67%	10.620%
12	7.625	2038	2048	2067	rBV2	32362	64272	9.40%	1.336%
13	8.091	2183	2193	2225	rBV3	179135	495450	72.44%	10.302%
14	8.249	2236	2242	2252	rVB9	5245	8717	1.27%	0.181%
15	8.850	2417	2429	2448	rBV	230948	388869	56.85%	8.086%
16	10.214	2842	2853	2872	rBV	92591	152094	22.24%	3.163%
17	11.249	3164	3175	3191	rBV	200402	322657	47.17%	6.709%
18	11.532	3249	3263	3280	rBV2	39759	73452	10.74%	1.527%
19	11.622	3280	3291	3308	rVB	248659	395644	57.85%	8.227%
20	12.345	3507	3516	3529	rVB7	11421	19257	2.82%	0.400%




Sum of corrected areas: 4809105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027659.D
Acq On : 01 Sep 2022 10:39
Operator : SY/MD
Sample : N4400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

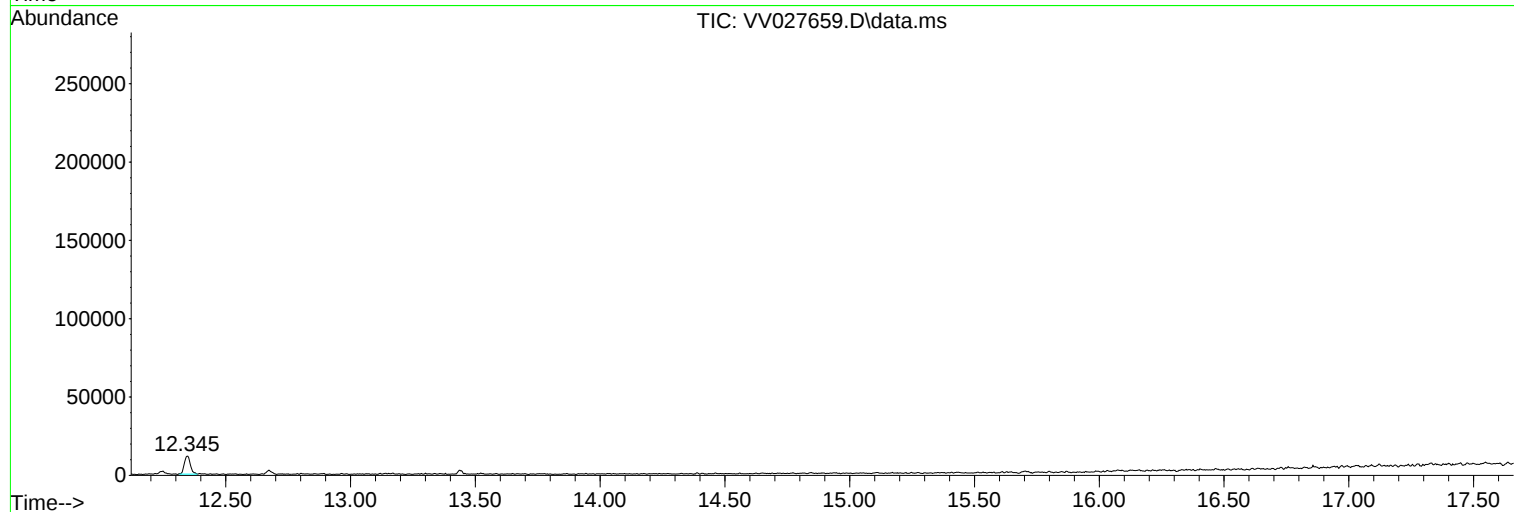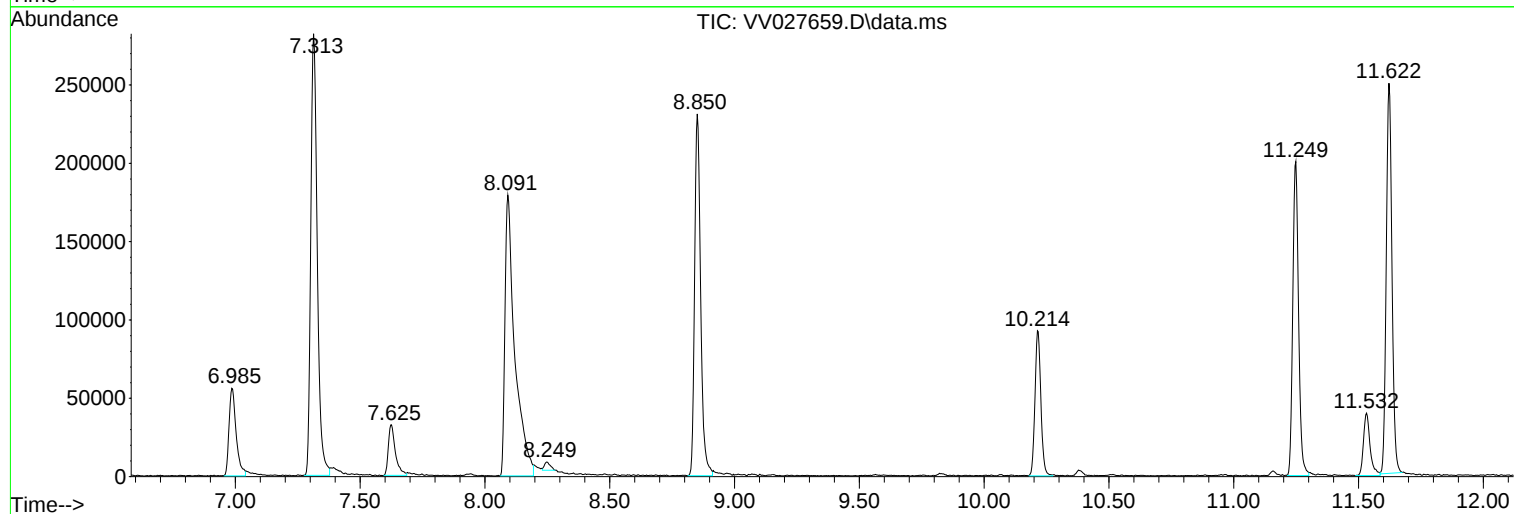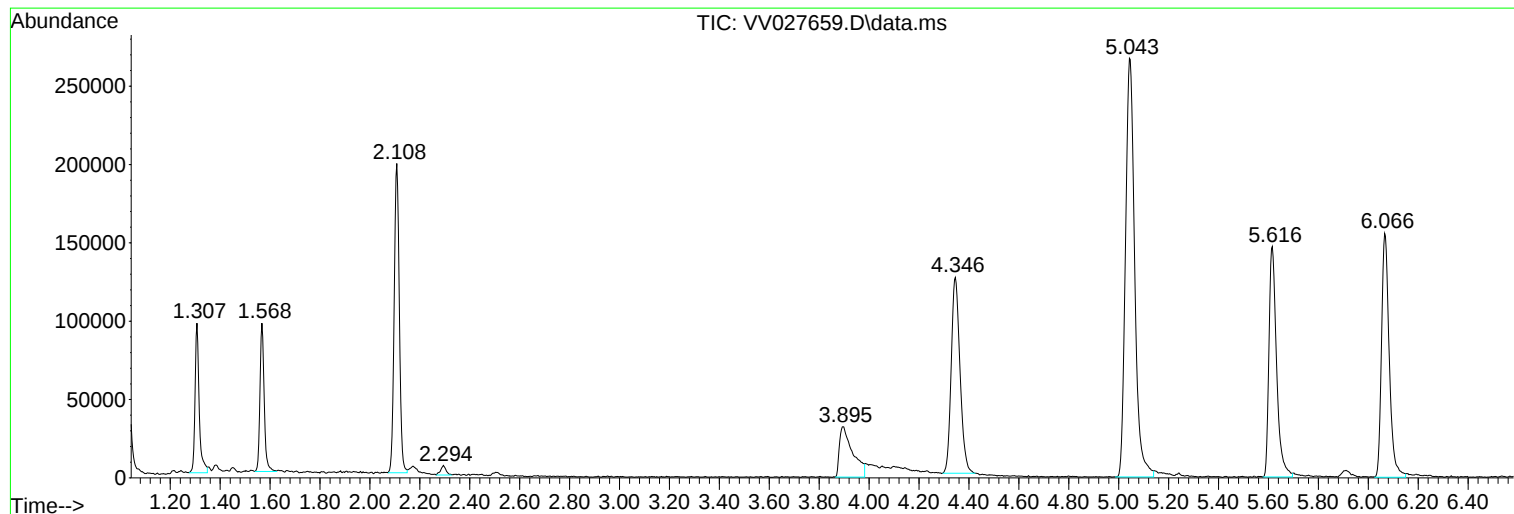

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027659.D
Acq On : 01 Sep 2022 10:39
Operator : SY/MD
Sample : N4400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVG6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.532	1.14 ug/L	73452	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
5	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64

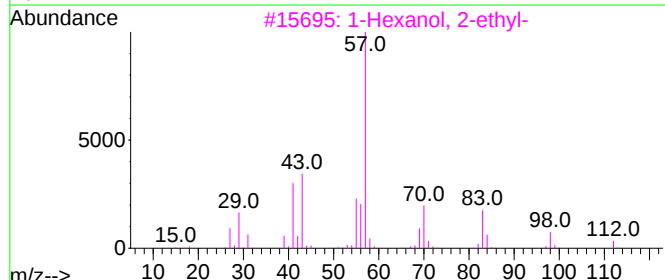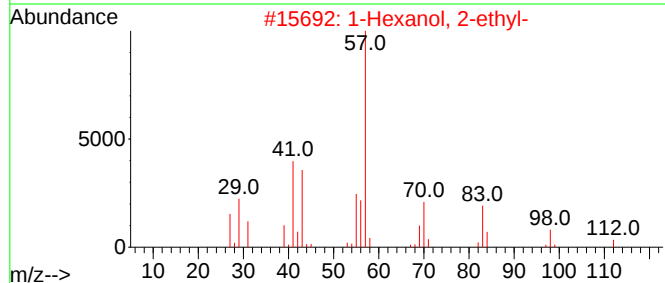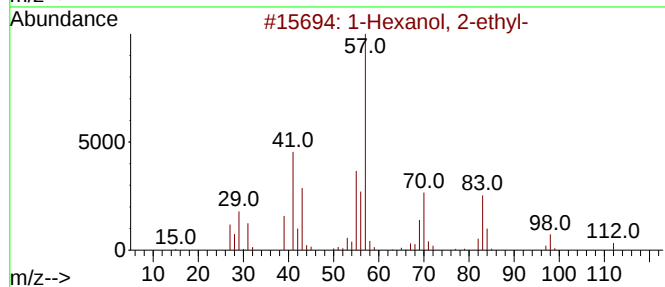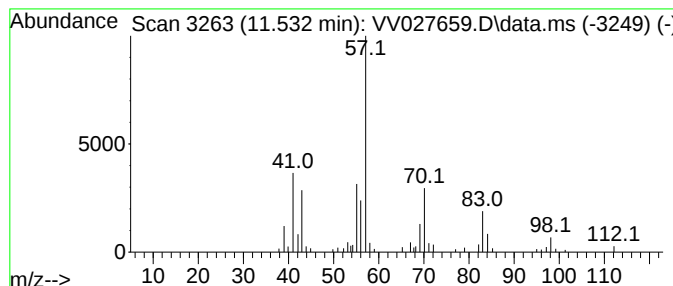

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027659.D
Acq On : 01 Sep 2022 10:39
Operator : SY/MD
Sample : N4400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.532	1.1	ug/L	73452	3	11.249	322657	5.0