

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027661.D
 Acq On : 01 Sep 2022 11:27
 Operator : SY/MD
 Sample : N4369-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	99	rBV	86865	104418	15.32%	2.089%
2	1.452	122	128	134	rVB4	7288	8217	1.21%	0.164%
3	1.568	154	164	176	rBV	89778	104817	15.38%	2.097%
4	2.108	320	332	360	rVB	177388	259423	38.06%	5.189%
5	3.889	877	886	912	rBV	36717	132270	19.41%	2.646%
6	4.346	1014	1028	1054	rVB	126880	318199	46.68%	6.365%
7	5.043	1228	1245	1270	rBV2	264741	681610	100.00%	13.633%
8	5.616	1409	1423	1452	rBV	152456	326165	47.85%	6.524%
9	5.908	1506	1514	1529	rBV8	3911	8452	1.24%	0.169%
10	6.066	1549	1563	1588	rBV	163150	343399	50.38%	6.869%
11	6.986	1838	1849	1873	rBV	54048	108850	15.97%	2.177%
12	7.313	1937	1951	1975	rBV	271671	490076	71.90%	9.802%
13	7.625	2037	2048	2068	rBV	32118	64079	9.40%	1.282%
14	7.973	2146	2156	2172	rVB2	84057	147156	21.59%	2.943%
15	8.092	2182	2193	2237	rBV2	206254	598831	87.86%	11.978%
16	8.850	2415	2429	2453	rBV	241657	409332	60.05%	8.187%
17	10.214	2842	2853	2872	rBV	102548	171028	25.09%	3.421%
18	11.246	3164	3174	3200	rBV	205420	330035	48.42%	6.601%
19	11.622	3278	3291	3312	rBV	242751	393216	57.69%	7.865%




Sum of corrected areas: 4999573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027661.D
Acq On : 01 Sep 2022 11:27
Operator : SY/MD
Sample : N4369-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

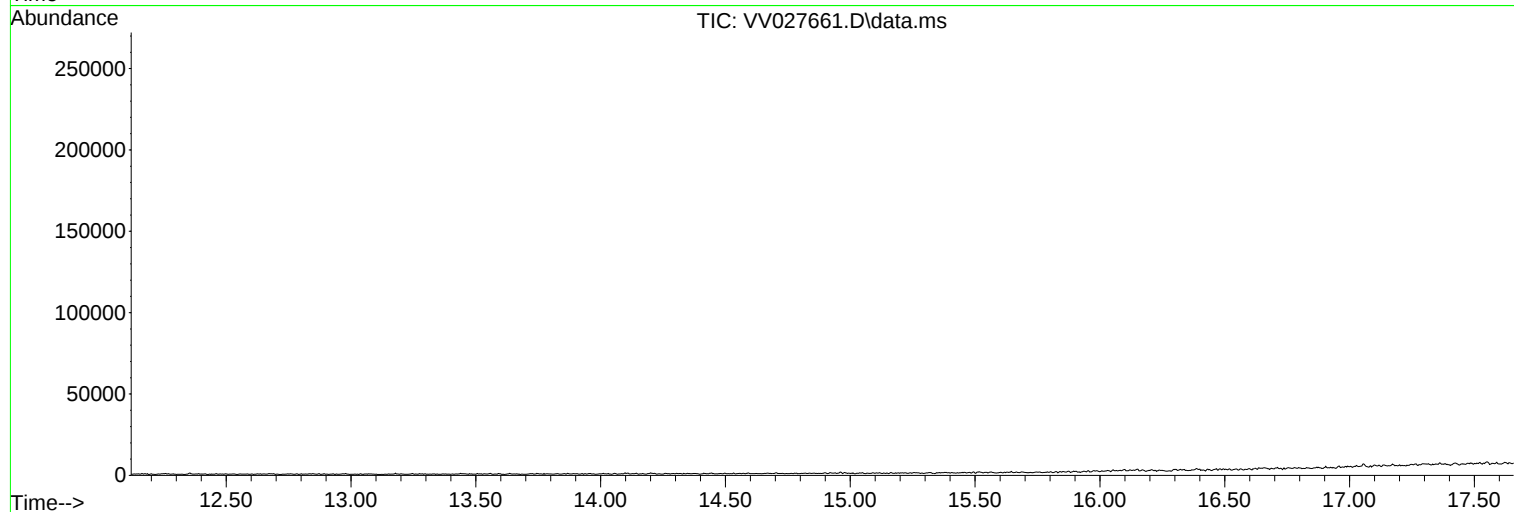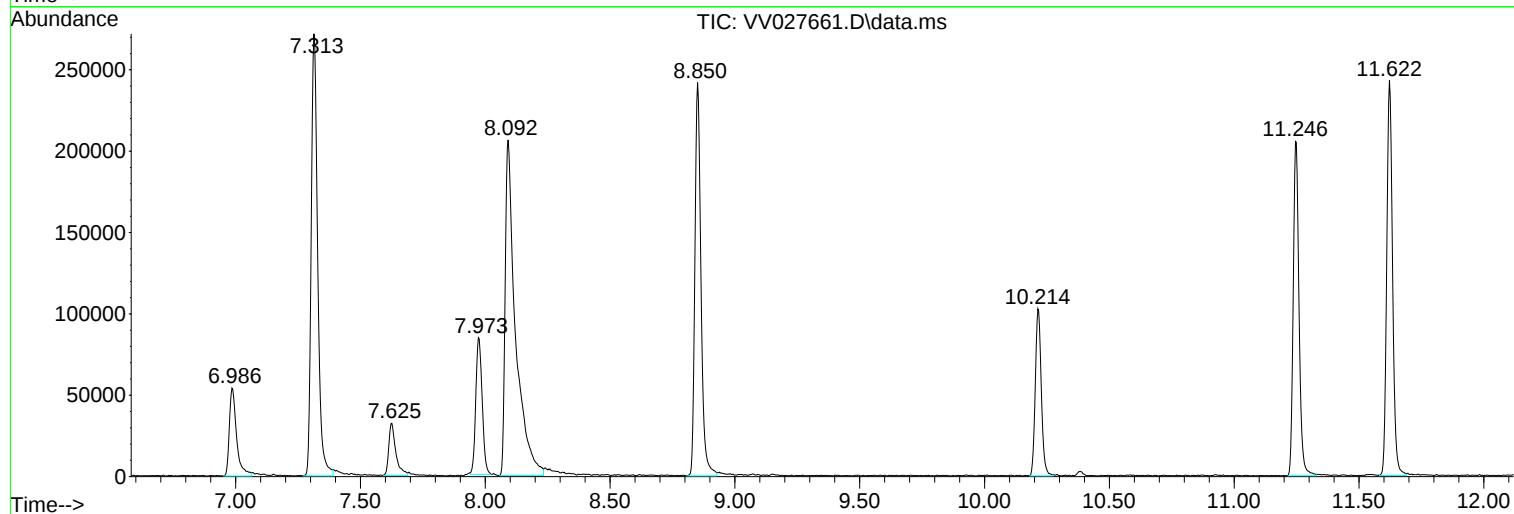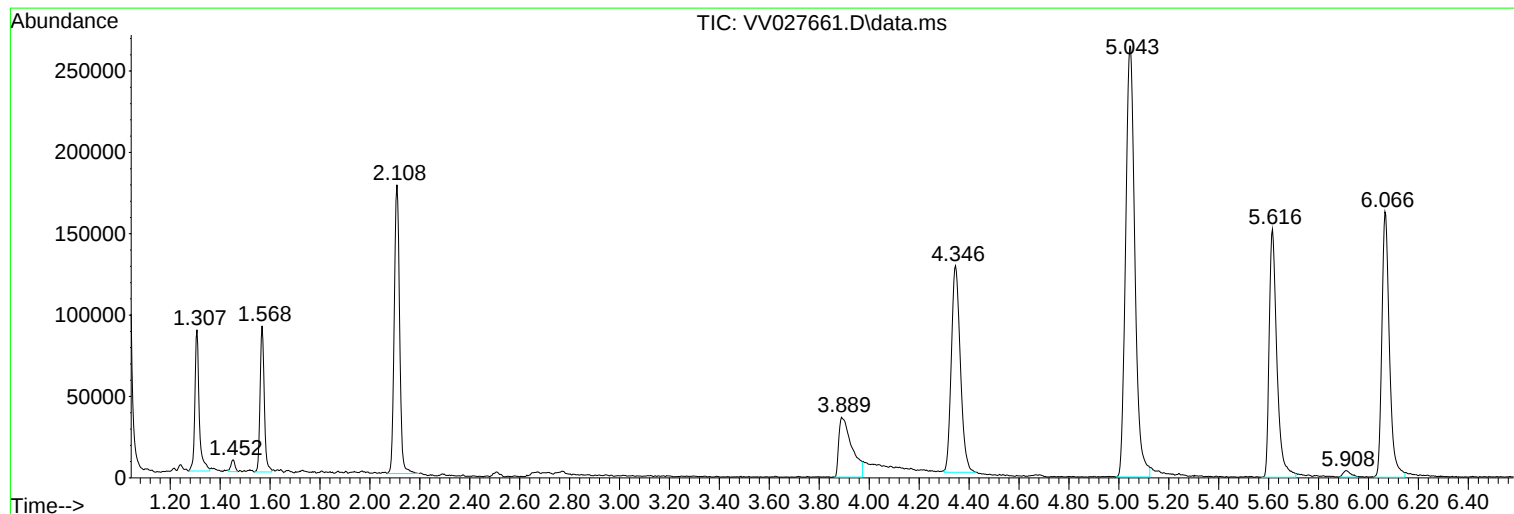

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027661.D
Acq On : 01 Sep 2022 11:27
Operator : SY/MD
Sample : N4369-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027661.D
Acq On : 01 Sep 2022 11:27
Operator : SY/MD
Sample : N4369-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc