

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027667.D
 Acq On : 01 Sep 2022 13:52
 Operator : SY/MD
 Sample : N4369-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	102	rBV	82873	99101	14.54%	1.914%
2	1.452	122	128	134	rVB2	7529	8254	1.21%	0.159%
3	1.568	156	164	176	rBV	85639	100342	14.73%	1.938%
4	2.108	321	332	356	rVB	171448	253385	37.19%	4.894%
5	2.767	520	537	555	rBV2	65497	142226	20.87%	2.747%
6	3.892	874	887	916	rBV	44343	180920	26.55%	3.495%
7	4.346	1011	1028	1056	rBV2	129374	330152	48.45%	6.377%
8	5.043	1229	1245	1275	rBV2	261499	681363	100.00%	13.161%
9	5.616	1411	1423	1457	rBV	152810	324682	47.65%	6.271%
10	5.918	1501	1517	1532	rBV8	23643	54747	8.03%	1.057%
11	6.066	1549	1563	1590	rBV	161565	347414	50.99%	6.711%
12	6.985	1835	1849	1877	rBV	54037	111247	16.33%	2.149%
13	7.313	1940	1951	1972	rBV	266480	484176	71.06%	9.352%
14	7.625	2038	2048	2068	rBV	31428	64007	9.39%	1.236%
15	7.976	2136	2157	2173	rBV4	43115	77427	11.36%	1.496%
16	8.092	2182	2193	2235	rBV2	236158	618020	90.70%	11.937%
17	8.850	2417	2429	2451	rBV	238740	406252	59.62%	7.847%
18	10.214	2842	2853	2868	rBV	106376	175324	25.73%	3.387%
19	11.246	3164	3174	3196	rBV	207969	324935	47.69%	6.276%
20	11.622	3279	3291	3314	rBV	247381	393157	57.70%	7.594%




Sum of corrected areas: 5177131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027667.D
Acq On : 01 Sep 2022 13:52
Operator : SY/MD
Sample : N4369-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

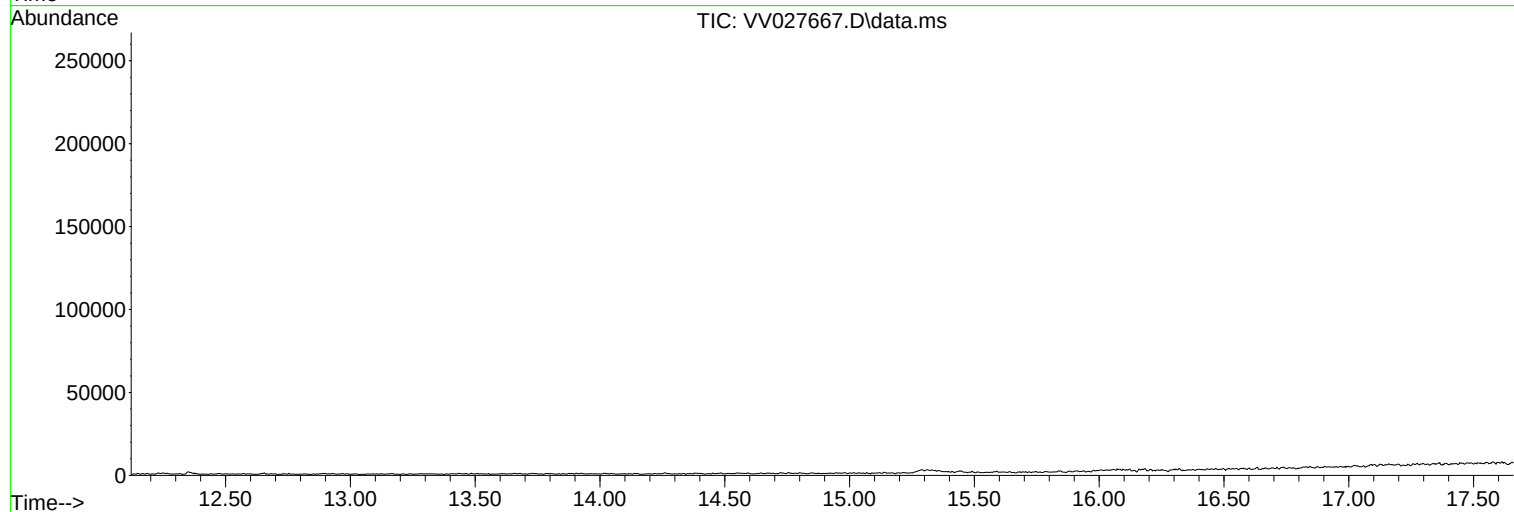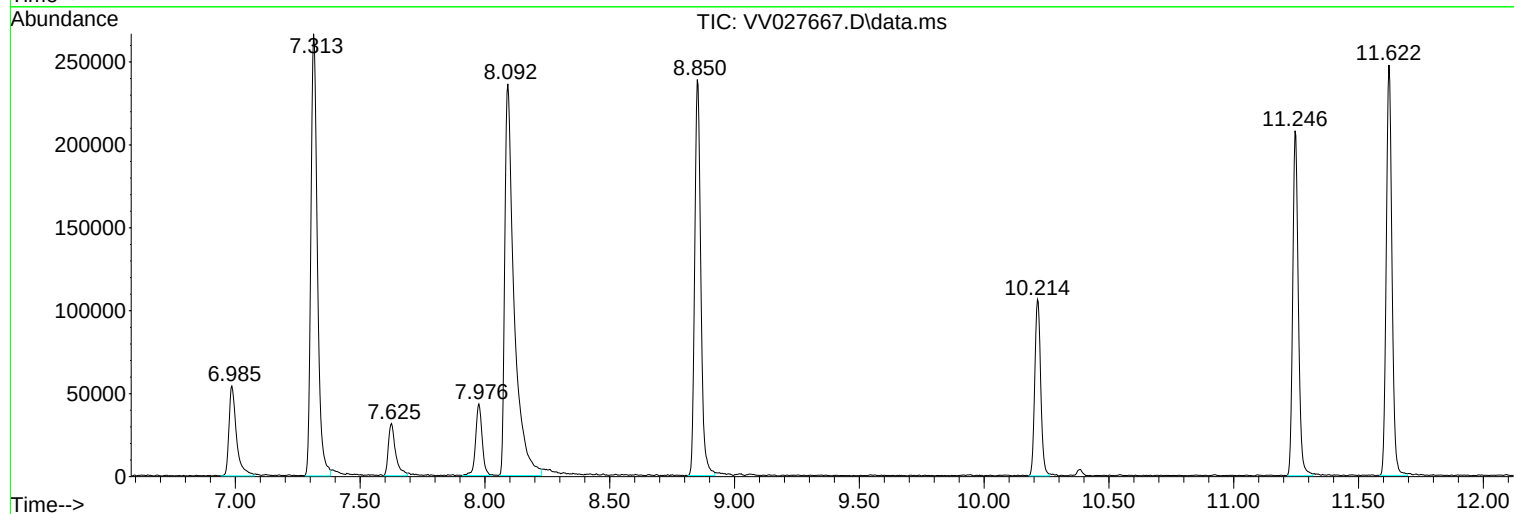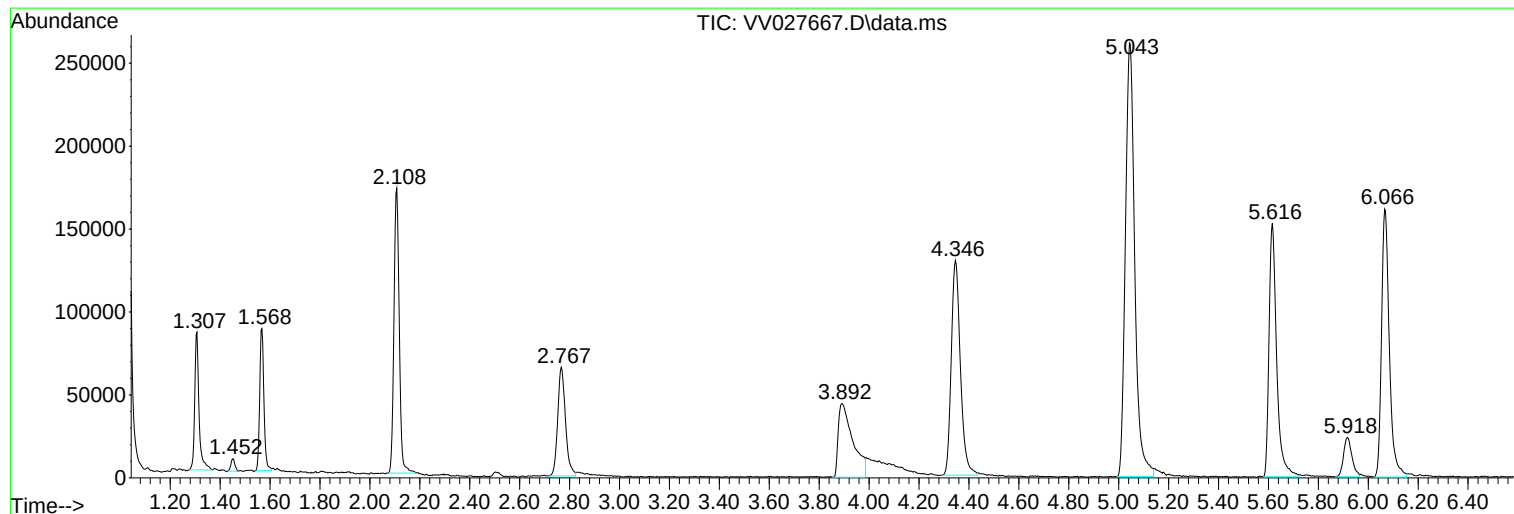

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027667.D
Acq On : 01 Sep 2022 13:52
Operator : SY/MD
Sample : N4369-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027667.D
Acq On : 01 Sep 2022 13:52
Operator : SY/MD
Sample : N4369-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc