

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027669.D
 Acq On : 01 Sep 2022 14:38
 Operator : SY/MD
 Sample : N4369-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	92	rBV	84934	100930	14.07%	1.837%
2	1.568	155	164	176	rBV	92284	107275	14.95%	1.952%
3	2.108	319	332	344	rBV	177445	258858	36.08%	4.711%
4	2.767	523	537	560	rBV2	25305	56768	7.91%	1.033%
5	3.899	878	889	921	rBV2	43573	180176	25.11%	3.279%
6	4.346	1012	1028	1059	rVB	134865	339170	47.27%	6.173%
7	5.047	1230	1246	1273	rBV2	277195	717542	100.00%	13.059%
8	5.619	1411	1424	1448	rBV2	151627	326197	45.46%	5.937%
9	5.918	1504	1517	1537	rBV5	49576	107939	15.04%	1.964%
10	6.069	1550	1564	1589	rBV2	169508	361082	50.32%	6.571%
11	6.989	1838	1850	1870	rBV2	55645	112427	15.67%	2.046%
12	7.317	1934	1952	1975	rBV	282898	518508	72.26%	9.436%
13	7.625	2037	2048	2065	rBV2	33698	64354	8.97%	1.171%
14	7.976	2144	2157	2173	rBV	158014	271846	37.89%	4.947%
15	8.092	2183	2193	2233	rBV2	235084	640320	89.24%	11.653%
16	8.850	2419	2429	2455	rBV	239403	409412	57.06%	7.451%
17	10.217	2842	2854	2873	rBV	110360	180415	25.14%	3.283%
18	11.249	3164	3175	3194	rBV	204462	325654	45.38%	5.927%
19	11.622	3279	3291	3308	rBV	257812	415855	57.96%	7.568%




Sum of corrected areas: 5494728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027669.D
Acq On : 01 Sep 2022 14:38
Operator : SY/MD
Sample : N4369-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

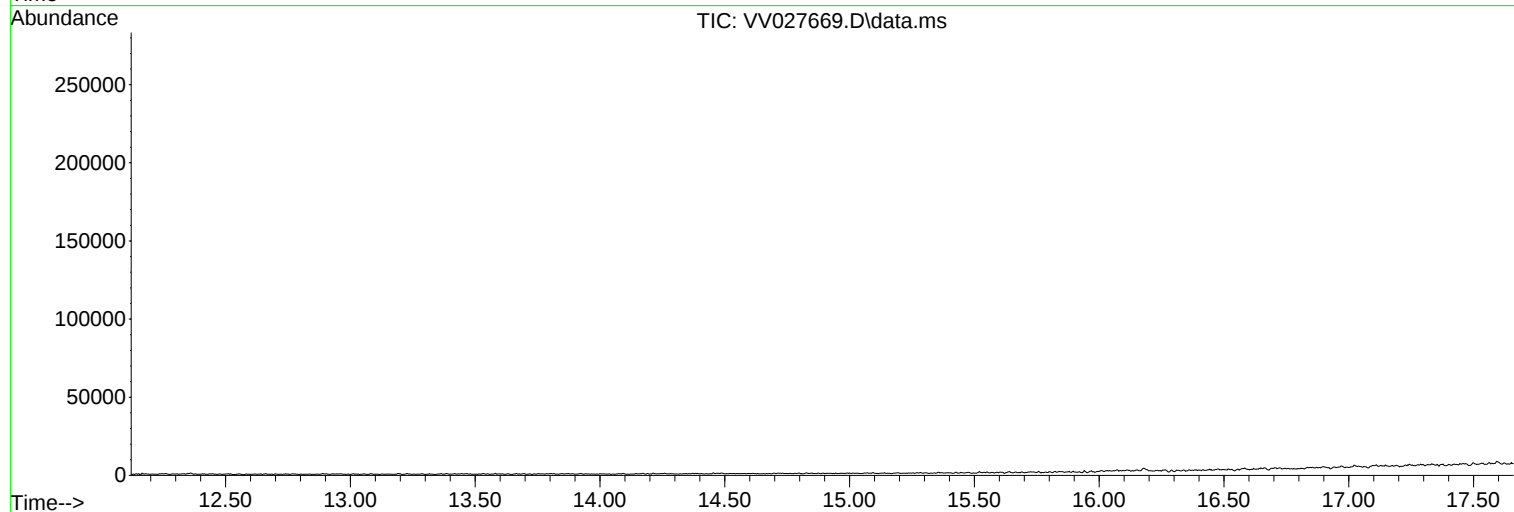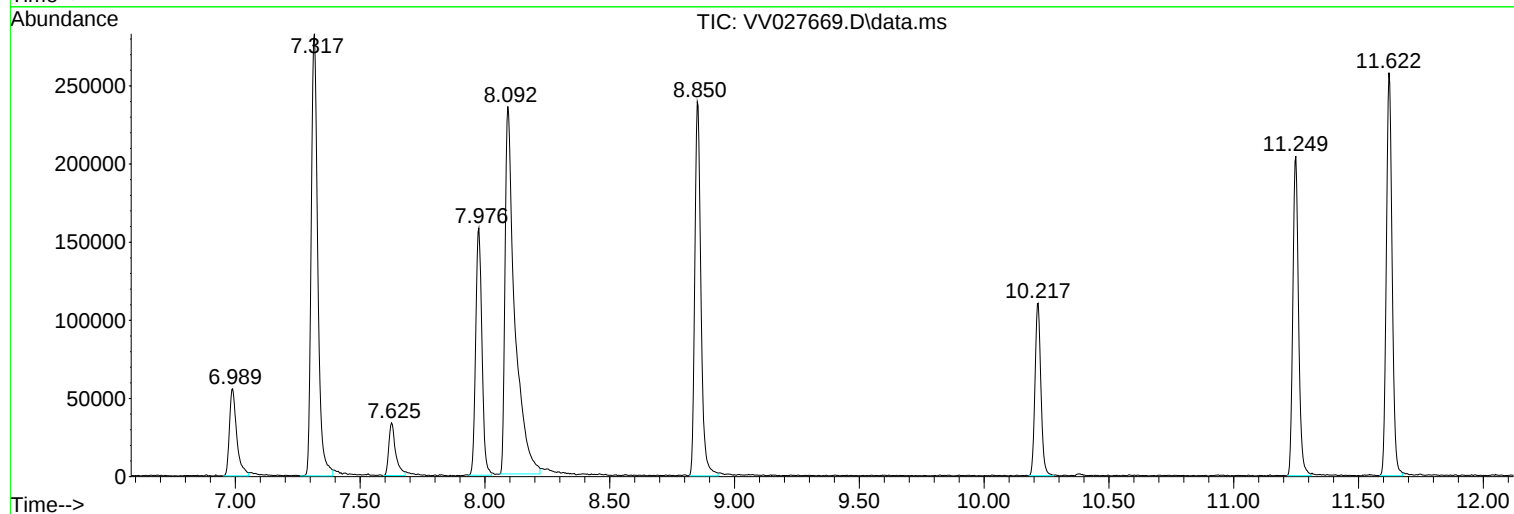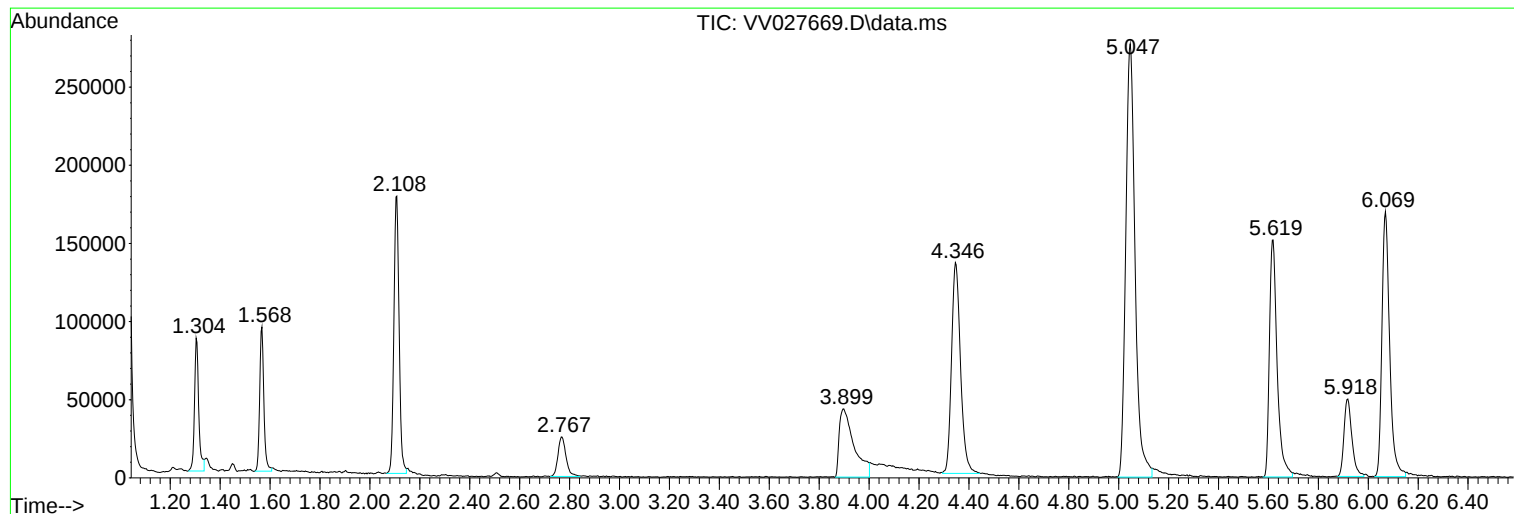

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027669.D
Acq On : 01 Sep 2022 14:38
Operator : SY/MD
Sample : N4369-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
Data File : VV027669.D
Acq On : 01 Sep 2022 14:38
Operator : SY/MD
Sample : N4369-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc