


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027611.D
 Acq On : 31 Aug 2022 10:21
 Operator : SY/MD
 Sample : BFB364
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB364

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Sep 01 02:33:10 2022

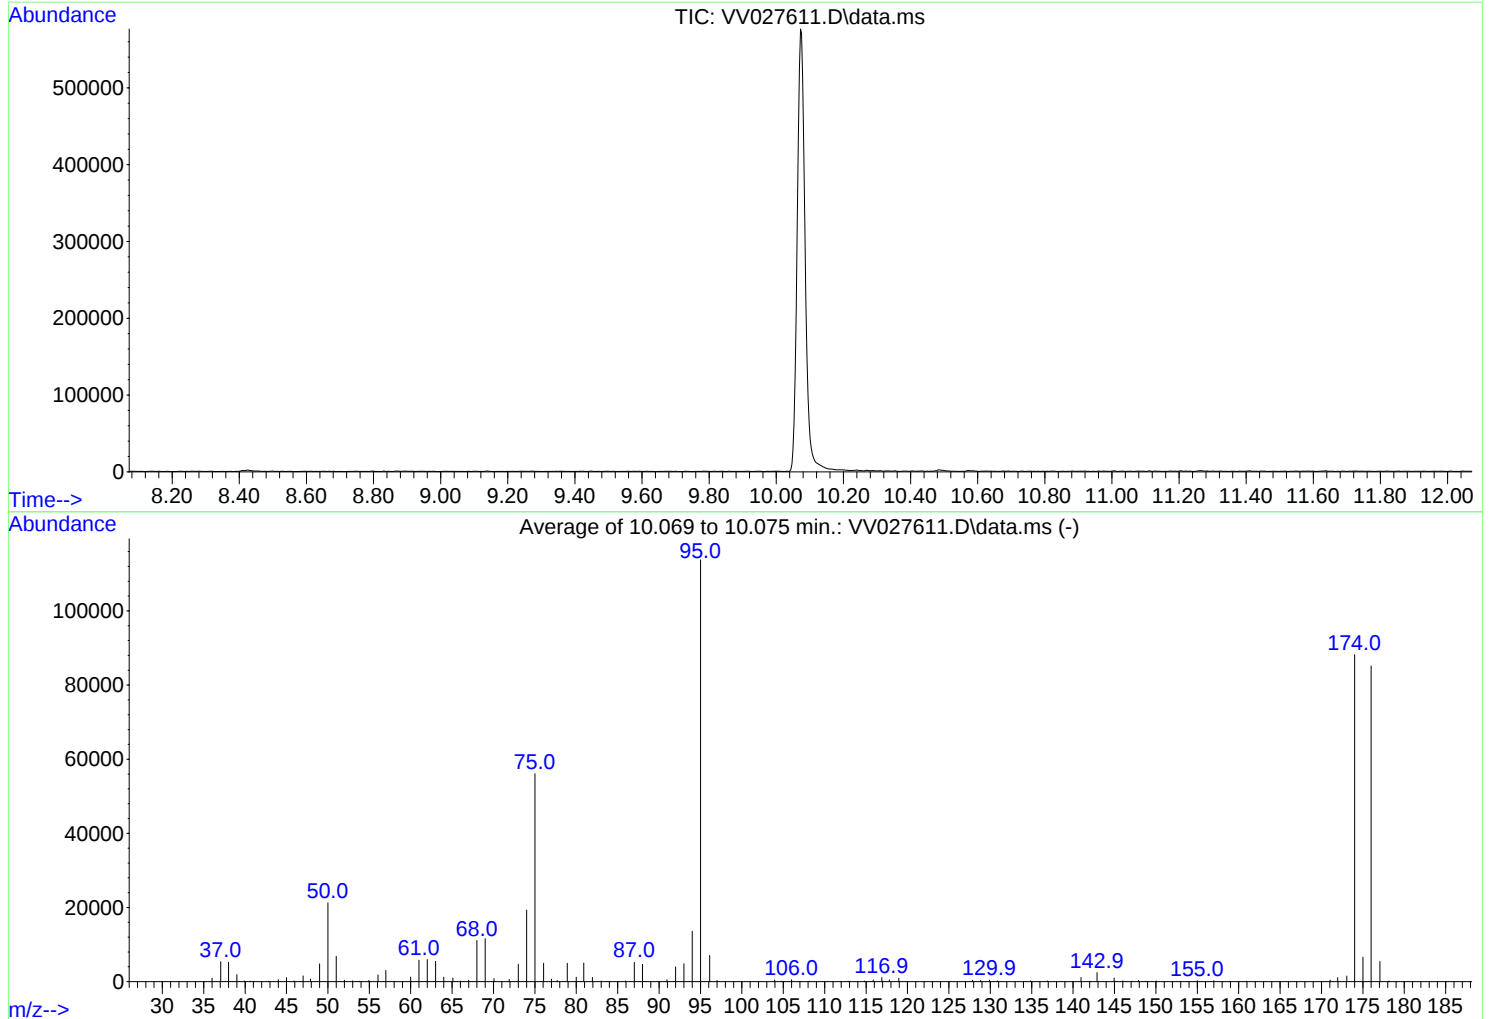

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	21285	PASS
75	95	30	80	49.3	56106	PASS
95	95	100	100	100.0	113781	PASS
96	95	5	9	6.2	7063	PASS
173	174	0.00	2	1.7	1517	PASS
174	95	50	120	77.5	88176	PASS
175	174	5	9	7.5	6590	PASS
176	174	95	105	96.6	85136	PASS
177	176	5	10	6.4	5420	PASS

Scan 2796 (10.030 min): VV027611.D\data.ms
BFB364

m/z	Abundance
39.10	110.0
39.90	161.0
44.00	431.0
75.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	841.0
37.10	5372.0
38.00	4956.0
39.00	1937.0
39.90	355.0
42.90	103.0
44.10	857.0
45.00	1117.0
45.90	229.0
47.00	1571.0
47.90	706.0
49.00	4460.0
50.00	20440.0
51.00	6702.0
52.00	339.0
53.00	188.0
53.80	115.0
55.00	341.0
56.00	1694.0
57.00	2990.0
57.90	139.0
60.00	1157.0
61.00	5619.0
62.00	5681.0
63.00	4986.0
64.00	1217.0
65.10	978.0
66.00	149.0
67.00	348.0
68.00	10846.0
69.00	10983.0
70.10	852.0
71.00	113.0
71.90	603.0
73.00	4490.0
74.00	18504.0
75.00	53224.0
76.00	5094.0
77.00	701.0
77.70	303.0
78.90	4702.0
80.00	1118.0
80.90	4696.0
82.00	1034.0
83.00	171.0
85.90	202.0
87.00	4644.0
88.00	4428.0
91.00	490.0
92.00	3783.0
93.00	4705.0
94.00	12755.0
95.00	107216.0
96.10	6888.0
97.00	297.0
104.00	385.0
104.80	186.0
106.00	518.0
106.80	159.0
108.20	105.0
110.90	141.0
112.80	135.0
114.80	148.0
115.90	475.0
116.90	1039.0
117.80	438.0
118.90	776.0
127.90	362.0
128.80	266.0
129.90	414.0
130.90	181.0
134.80	196.0
136.90	224.0
140.00	101.0
140.90	988.0
142.00	139.0
142.90	2289.0
145.00	845.0
146.00	245.0
147.10	132.0
147.90	262.0
148.70	109.0
150.10	141.0
152.90	139.0
155.00	253.0
157.00	250.0
158.90	123.0
160.90	106.0
171.00	439.0
172.00	1063.0
173.00	1369.0
174.00	82208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

175.00	6352.0
176.00	78584.0
177.10	4998.0
178.20	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	942.0
37.10	5602.0
38.00	5339.0
39.00	2073.0
39.90	396.0
40.60	209.0
42.80	130.0
44.00	986.0
45.00	1125.0
45.90	223.0
47.00	1562.0
47.90	719.0
49.00	4965.0
50.00	21984.0
51.00	7089.0
52.00	415.0
53.00	220.0
53.80	149.0
55.00	351.0
56.00	1867.0
57.00	3134.0
58.00	120.0
60.00	1307.0
61.00	5970.0
62.00	6187.0
63.00	5789.0
64.00	1271.0
65.10	1035.0
66.00	177.0
67.00	328.0
68.00	11440.0
69.00	11992.0
70.10	846.0
71.00	108.0
71.90	628.0
73.00	4829.0
74.00	20056.0
75.00	58240.0
76.10	5033.0
77.00	749.0
77.70	311.0
78.90	5104.0
80.00	1243.0
80.90	5074.0
81.90	1141.0
83.00	219.0
86.00	209.0
87.00	5413.0
88.00	4806.0
91.00	576.0
92.00	4126.0
93.00	4929.0
94.00	14091.0
95.00	117616.0
96.10	7320.0
97.00	308.0
103.90	476.0
104.80	169.0
106.00	503.0
106.80	149.0
108.20	117.0
110.90	120.0
111.90	135.0
112.90	128.0
114.80	182.0
115.80	524.0
116.90	1108.0
117.80	493.0
118.90	879.0
127.90	410.0
128.80	307.0
129.90	432.0
130.80	227.0
134.80	237.0
136.90	225.0
140.90	1151.0
142.00	149.0
142.90	2540.0
145.00	1015.0
146.00	231.0
147.10	158.0
147.90	319.0
148.80	113.0
150.00	167.0
153.00	145.0
155.00	265.0
157.00	249.0
158.90	113.0
161.00	149.0
171.10	456.0
172.00	1142.0
173.10	1584.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

174.00	91152.0
175.00	6775.0
176.00	88088.0
177.00	5580.0
178.20	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

m/z	Abundance
36.00	1041.0
37.00	5227.0
38.00	5338.0
39.00	2026.0
39.90	346.0
40.60	229.0
42.80	124.0
44.00	1033.0
45.00	988.0
45.90	184.0
47.00	1514.0
47.90	704.0
49.00	4971.0
50.00	21432.0
51.00	6703.0
52.00	445.0
53.00	205.0
53.90	168.0
54.10	168.0
54.90	365.0
56.10	1847.0
57.00	2987.0
58.10	101.0
60.00	1281.0
61.00	5818.0
62.00	6057.0
63.00	5725.0
64.00	1111.0
65.10	963.0
66.00	183.0
67.00	323.0
68.00	10943.0
69.00	11891.0
70.00	814.0
71.90	570.0
73.00	4847.0
74.00	19288.0
75.00	57208.0
76.00	4732.0
77.00	673.0
77.70	366.0
78.90	5060.0
80.00	1301.0
80.90	5265.0
81.90	1191.0
83.00	188.0
86.00	216.0
87.00	5484.0
88.00	4697.0
90.90	550.0
92.00	3964.0
93.00	4929.0
94.00	13973.0
95.00	116512.0
96.10	6981.0
97.00	262.0
103.90	500.0
105.10	167.0
106.00	495.0
107.10	159.0
108.00	113.0
111.90	135.0
112.90	118.0
114.80	201.0
115.80	478.0
116.90	1109.0
117.80	490.0
119.00	916.0
127.80	457.0
128.90	336.0
129.90	424.0
130.80	271.0
134.90	249.0
136.90	213.0
141.00	1209.0
142.10	157.0
142.90	2512.0
144.90	1111.0
146.00	210.0
147.10	164.0
147.90	340.0
148.90	129.0
150.00	171.0
153.00	142.0
153.80	113.0
155.00	263.0
157.00	257.0
161.00	157.0
171.10	464.0
171.90	1065.0
173.10	1598.0
174.00	91168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364

175.00	6644.0
176.00	88736.0
177.00	5683.0
178.10	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB364