


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083122\
 Data File : VV027621.D
 Acq On : 31 Aug 2022 16:42
 Operator : SY/MD
 Sample : BFB365
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB365

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 03 05:30:57 2022

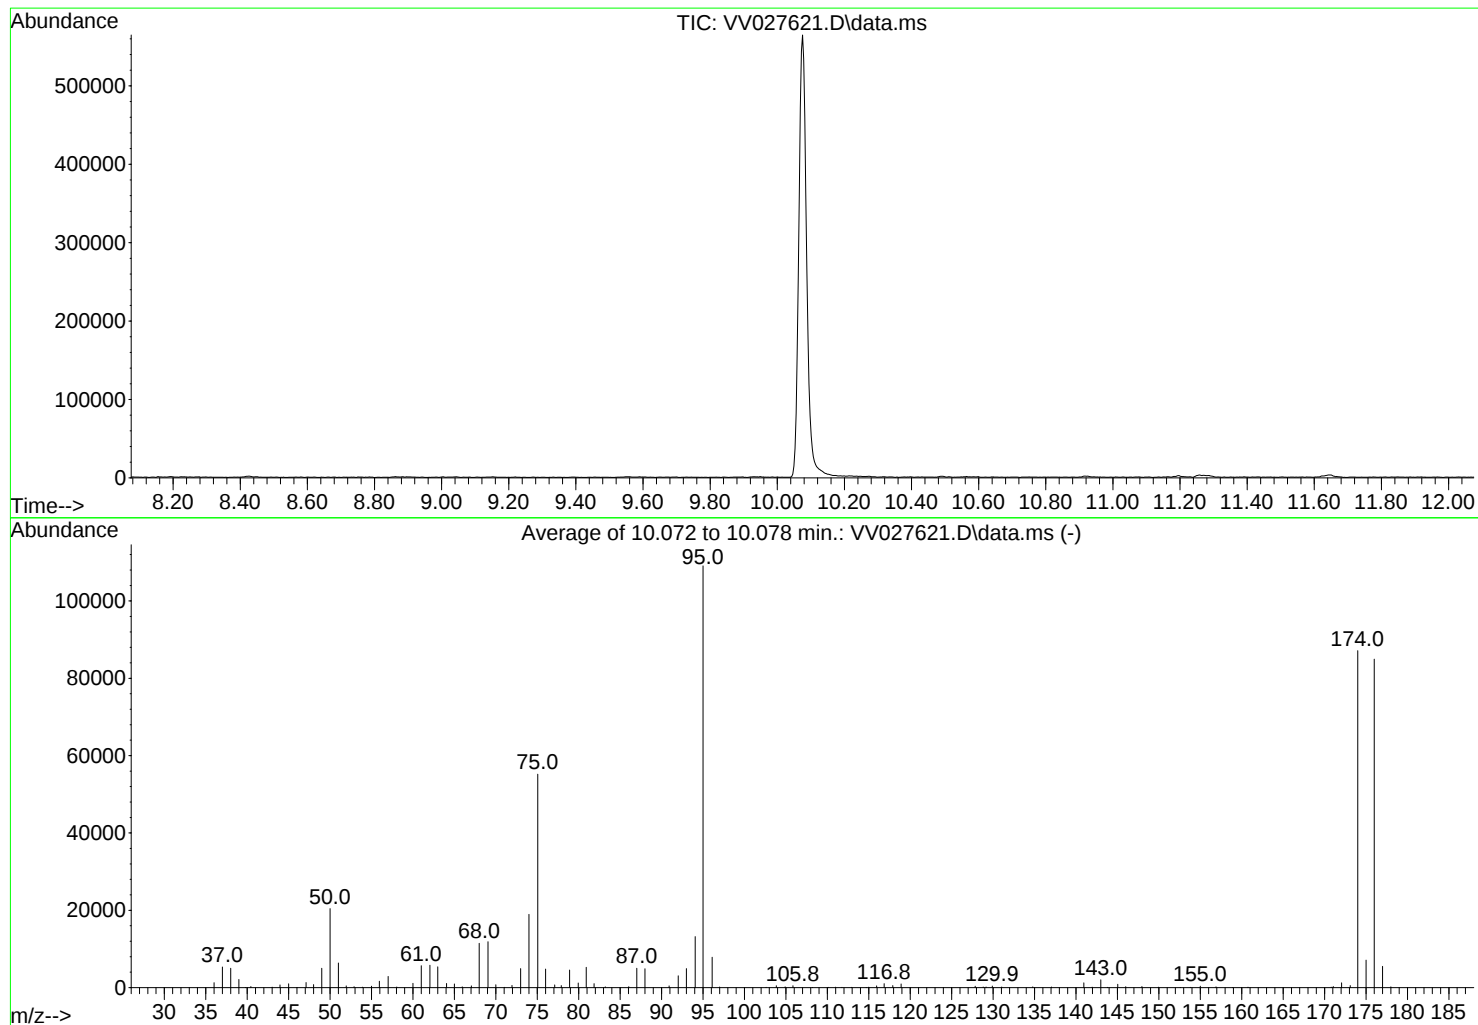

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	20440	PASS
75	95	30	80	50.6	55200	PASS
95	95	100	100	100.0	109080	PASS
96	95	5	9	7.2	7865	PASS
173	174	0.00	2	0.6	547	PASS
174	95	50	120	79.9	87125	PASS
175	174	5	9	8.2	7125	PASS
176	174	95	105	97.5	84933	PASS
177	176	5	10	6.5	5499	PASS

m/z	Abundance
37.00	122.0
39.80	214.0
40.10	215.0
44.00	356.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	1274.0
37.10	5425.0
38.00	5164.0
39.00	2168.0
39.80	374.0
40.40	258.0
43.00	128.0
44.00	1088.0
45.00	987.0
46.00	167.0
47.20	1398.0
48.00	822.0
49.00	4822.0
50.00	21000.0
51.00	6368.0
51.90	506.0
52.90	180.0
53.80	134.0
55.00	411.0
56.00	1674.0
57.00	2963.0
58.00	169.0
60.00	1186.0
61.00	5372.0
62.00	5621.0
63.00	5406.0
64.10	1098.0
65.00	898.0
65.90	244.0
67.00	455.0
68.00	11412.0
69.00	11947.0
70.00	789.0
71.00	135.0
71.90	610.0
73.00	5077.0
74.00	19096.0
75.10	54872.0
76.00	4914.0
77.00	780.0
77.90	482.0
78.90	4465.0
79.90	1178.0
80.90	5180.0
81.90	1005.0
83.20	203.0
86.10	233.0
87.00	4933.0
88.00	4832.0
91.00	496.0
92.00	2955.0
93.00	4955.0
94.00	13068.0
95.00	110040.0
96.10	7992.0
97.00	163.0
103.90	503.0
104.90	175.0
105.80	548.0
110.10	127.0
111.00	147.0
114.70	120.0
115.00	120.0
116.00	447.0
116.90	1032.0
118.00	542.0
118.90	895.0
124.00	107.0
127.80	359.0
128.80	233.0
129.90	485.0
131.10	174.0
134.90	202.0
137.00	174.0
140.90	1197.0
143.00	1962.0
145.10	784.0
146.00	271.0
148.00	265.0
150.00	157.0
152.60	100.0
155.00	331.0
156.90	228.0
160.80	147.0
170.80	342.0
172.10	1070.0
174.00	85512.0
175.00	7147.0
176.00	82992.0
177.00	5465.0
178.00	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	1344.0
37.00	5599.0
38.00	5169.0
39.00	2138.0
39.80	405.0
40.50	295.0
43.00	124.0
44.00	1094.0
45.00	1002.0
47.10	1290.0
48.00	829.0
49.00	5177.0
50.00	21144.0
51.00	6489.0
52.00	485.0
52.90	258.0
53.90	110.0
55.00	408.0
55.90	1720.0
57.00	2938.0
58.10	152.0
60.00	1121.0
61.00	5978.0
62.00	6033.0
63.00	5566.0
64.10	1067.0
65.00	998.0
66.00	199.0
67.10	466.0
68.00	11873.0
69.10	12427.0
70.00	797.0
71.10	131.0
72.00	638.0
73.00	5128.0
74.00	19536.0
75.10	56680.0
76.00	4940.0
77.10	697.0
77.90	564.0
78.90	4629.0
79.90	1188.0
80.90	5443.0
81.90	1079.0
83.20	210.0
86.00	253.0
87.00	5172.0
88.00	5136.0
90.90	476.0
92.00	3157.0
93.00	5060.0
94.10	13489.0
95.00	112472.0
96.10	8167.0
97.00	175.0
102.60	124.0
103.80	508.0
104.90	189.0
105.90	528.0
110.10	110.0
111.00	147.0
111.70	103.0
112.90	115.0
115.00	153.0
115.90	454.0
116.90	1097.0
117.90	566.0
118.90	1008.0
127.90	374.0
128.80	226.0
129.10	226.0
129.90	417.0
131.10	172.0
134.80	208.0
137.10	178.0
140.90	1324.0
141.90	160.0
143.00	2102.0
143.80	120.0
145.00	845.0
146.00	285.0
147.90	295.0
150.00	146.0
153.80	122.0
155.00	396.0
156.90	223.0
160.80	135.0
171.00	376.0
172.00	1293.0
174.00	89848.0
175.00	7340.0
176.00	87920.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

177.005666.0

178.00238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
36.00	1173.0
37.00	5373.0
38.00	4646.0
39.00	1974.0
40.50	274.0
43.00	129.0
43.90	1057.0
45.00	963.0
47.00	1239.0
48.00	711.0
49.00	5010.0
50.00	19176.0
51.00	6239.0
52.00	432.0
52.90	311.0
54.00	123.0
55.00	333.0
56.00	1634.0
57.00	2856.0
58.10	131.0
60.00	1070.0
61.00	5708.0
62.10	5707.0
63.00	5219.0
64.00	1061.0
65.00	989.0
66.00	147.0
67.10	443.0
68.00	11155.0
69.10	11281.0
70.00	711.0
71.90	549.0
73.00	4570.0
74.00	18216.0
75.00	54048.0
76.00	4527.0
77.20	622.0
77.90	574.0
78.90	4550.0
80.00	1194.0
80.90	5151.0
81.80	1052.0
83.20	151.0
86.00	268.0
87.00	4901.0
88.00	4753.0
90.80	373.0
92.00	3099.0
93.00	4802.0
94.10	13013.0
95.00	104728.0
96.10	7437.0
97.00	188.0
102.60	119.0
103.90	494.0
104.90	209.0
105.90	458.0
108.20	102.0
111.00	119.0
111.80	140.0
112.90	155.0
115.00	156.0
115.90	429.0
116.80	1025.0
117.80	516.0
118.90	968.0
127.90	384.0
129.20	237.0
129.90	395.0
131.00	169.0
134.70	178.0
137.00	165.0
141.00	1179.0
142.00	166.0
143.00	1989.0
143.80	106.0
145.00	941.0
146.00	230.0
147.90	301.0
149.90	136.0
153.80	122.0
155.00	404.0
156.90	213.0
158.90	110.0
160.70	136.0
171.10	456.0
172.00	1374.0
173.10	1641.0
174.00	86016.0
175.00	6887.0
176.00	83888.0
177.00	5365.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

178.00

205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365