

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083123\
 Data File : VW031961.D
 Acq On : 31 Aug 2023 15:09
 Operator : SY/MD
 Sample : 04175-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP0

Quant Time: Sep 01 02:10:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 01 00:57:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	244871	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	233187	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	124150	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	85447	55.757	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 111.520%			
7) Chloroethane-d5	1.532	69	69879	52.016	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 104.040%			
11) 1,1-Dichloroethene-d2	2.063	65	36047	50.233	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.460%			
21) 2-Butanone-d5	3.793	46	117776	97.715	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 97.720%			
24) Chloroform-d	4.256	84	150489	44.927	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 89.860%			
26) 1,2-Dichloroethane-d4	4.947	65	101535	45.676	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 91.360%			
32) Benzene-d6	4.963	84	326660	51.338	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.680%			
36) 1,2-Dichloropropane-d6	5.992	67	103705	50.636	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 101.280%			
41) Toluene-d8	7.246	98	300993	51.339	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.680%			
43) trans-1,3-Dichloroprop...	7.558	79	50501	47.575	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 95.140%			
47) 2-Hexanone-d5	8.030	63	75934	120.969	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 120.970%			
56) 1,1,2,2-Tetrachloroeth...	10.156	84	128249	48.459	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 96.920%			
66) 1,2-Dichlorobenzene-d4	11.564	152	109175	48.239	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 96.480%			
Target Compounds					Qvalue	
13) Acetone	2.121	43	9162	8.540	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031961.D
Acq On : 31 Aug 2023 15:09
Operator : SY/MD
Sample : 04175-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYPO

Quant Time: Sep 01 02:10:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 01 00:57:38 2023
Response via : Initial Calibration

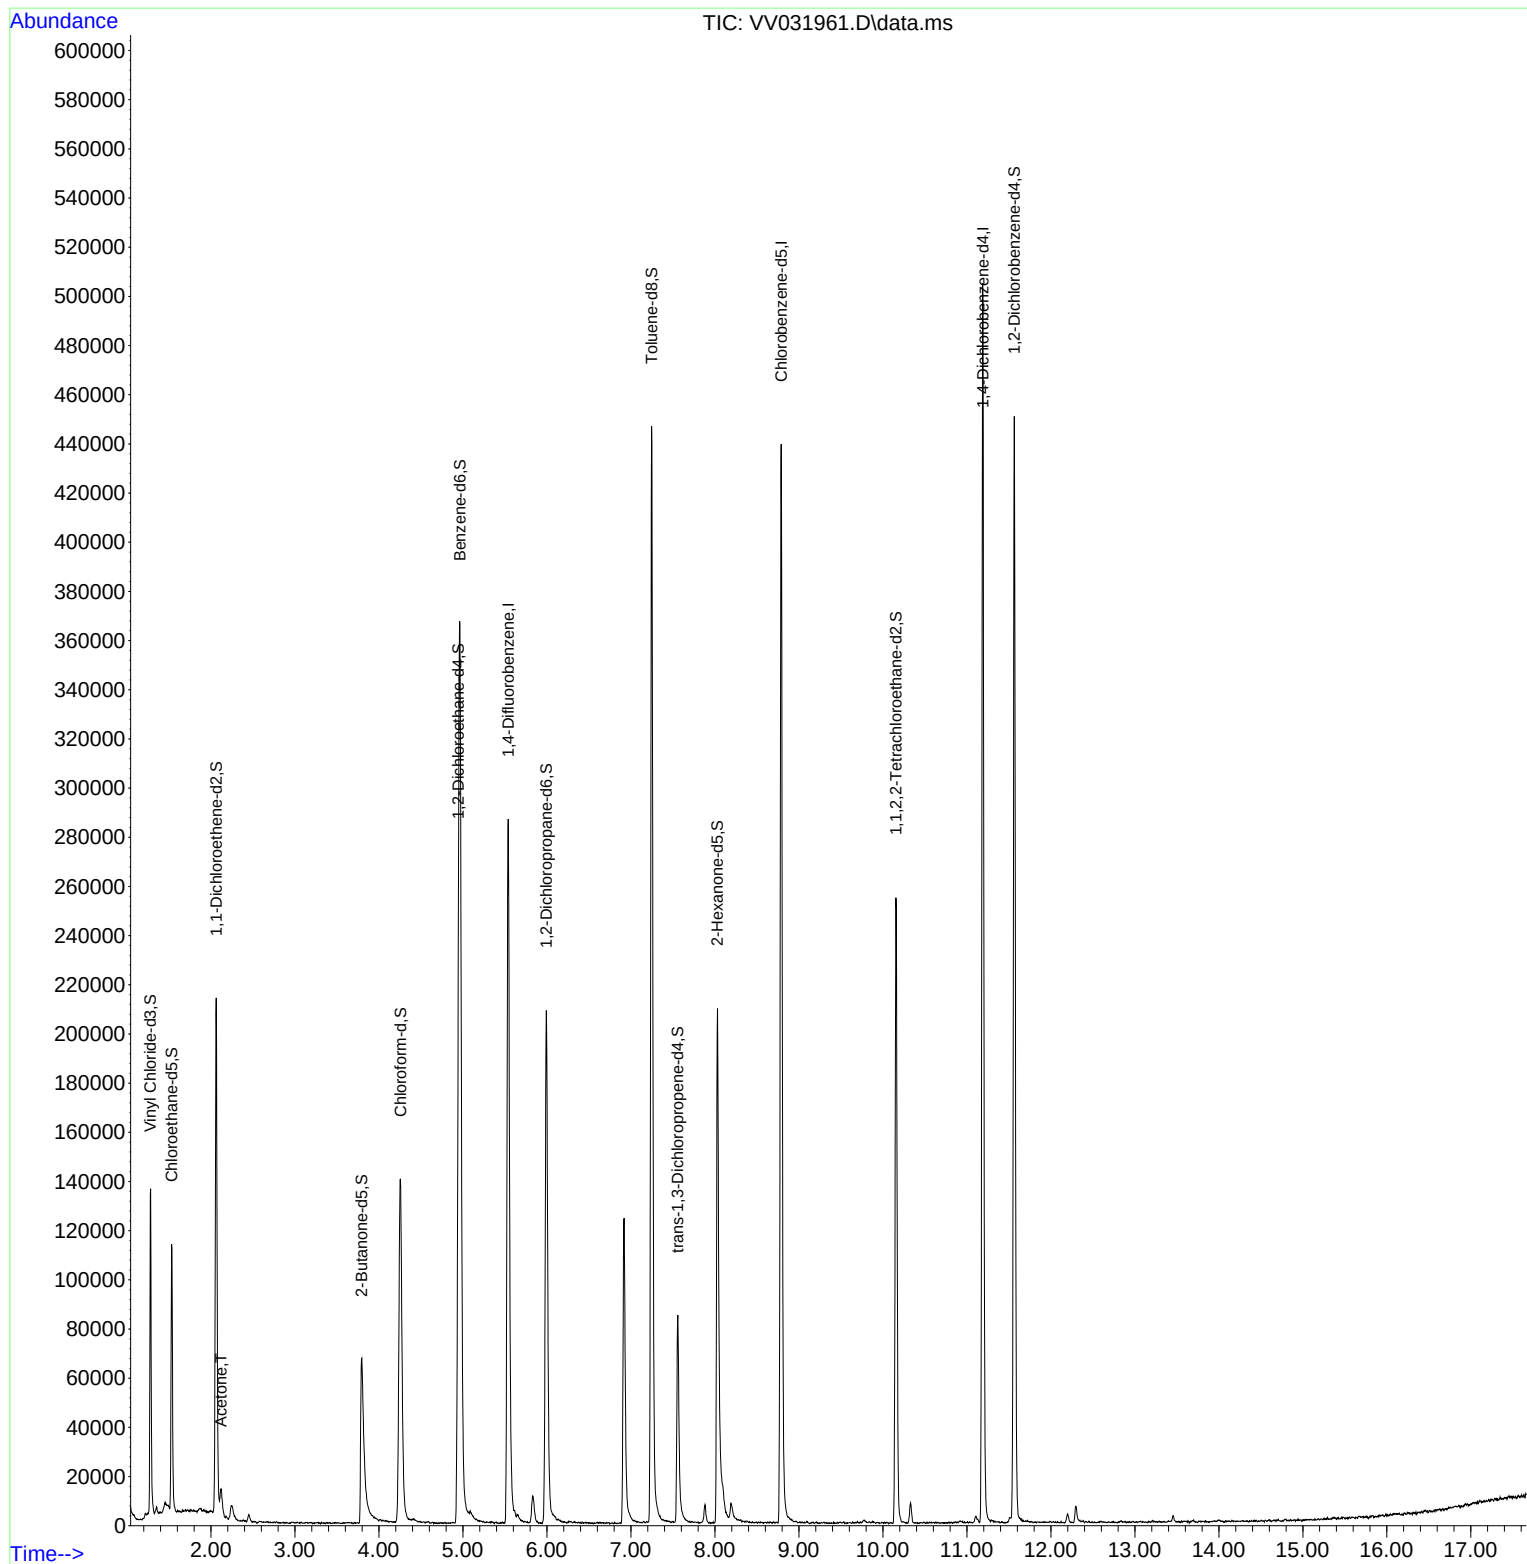

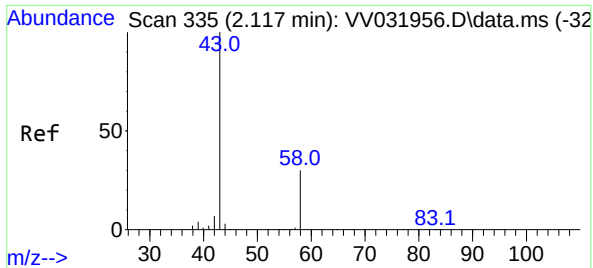

#13
Acetone
Concen: 8.540 ug/L
RT: 2.121 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV031961.D
Acq: 31 Aug 2023 15:09

Instrument :
MSVOA_V
ClientSampleId :
EZYPO

Tgt Ion: 43 Resp: 9162
Ion Ratio Lower Upper
43 100
58 30.2 0.0 61.0

