

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083123\
 Data File : VW031962.D
 Acq On : 31 Aug 2023 15:31
 Operator : SY/MD
 Sample : 04175-24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR5

Quant Time: Sep 01 02:10:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 01 00:57:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	257007	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	248090	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	132077	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	87571	54.445	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 108.880%			
7) Chloroethane-d5	1.532	69	69085	48.997	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 98.000%			
11) 1,1-Dichloroethene-d2	2.063	65	36701	48.730	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.460%			
21) 2-Butanone-d5	3.793	46	118818	93.925	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 93.920%			
24) Chloroform-d	4.256	84	152577	43.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 86.800%			
26) 1,2-Dichloroethane-d4	4.947	65	102678	44.010	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 88.020%			
32) Benzene-d6	4.966	84	330993	48.894	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 97.780%			
36) 1,2-Dichloropropane-d6	5.992	67	106262	48.768	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 97.540%			
41) Toluene-d8	7.249	98	300414	48.162	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 96.320%			
43) trans-1,3-Dichloroprop...	7.558	79	52552	46.533	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.060%			
47) 2-Hexanone-d5	8.030	63	79719	119.370	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 119.370%			
56) 1,1,2,2-Tetrachloroeth...	10.156	84	127513	45.287	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 90.580%			
66) 1,2-Dichlorobenzene-d4	11.564	152	113611	47.187	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 94.380%			
Target Compounds					Qvalue	
13) Acetone	2.117	43	8241	7.319	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031962.D
Acq On : 31 Aug 2023 15:31
Operator : SY/MD
Sample : 04175-24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR5

Quant Time: Sep 01 02:10:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 01 00:57:38 2023
Response via : Initial Calibration

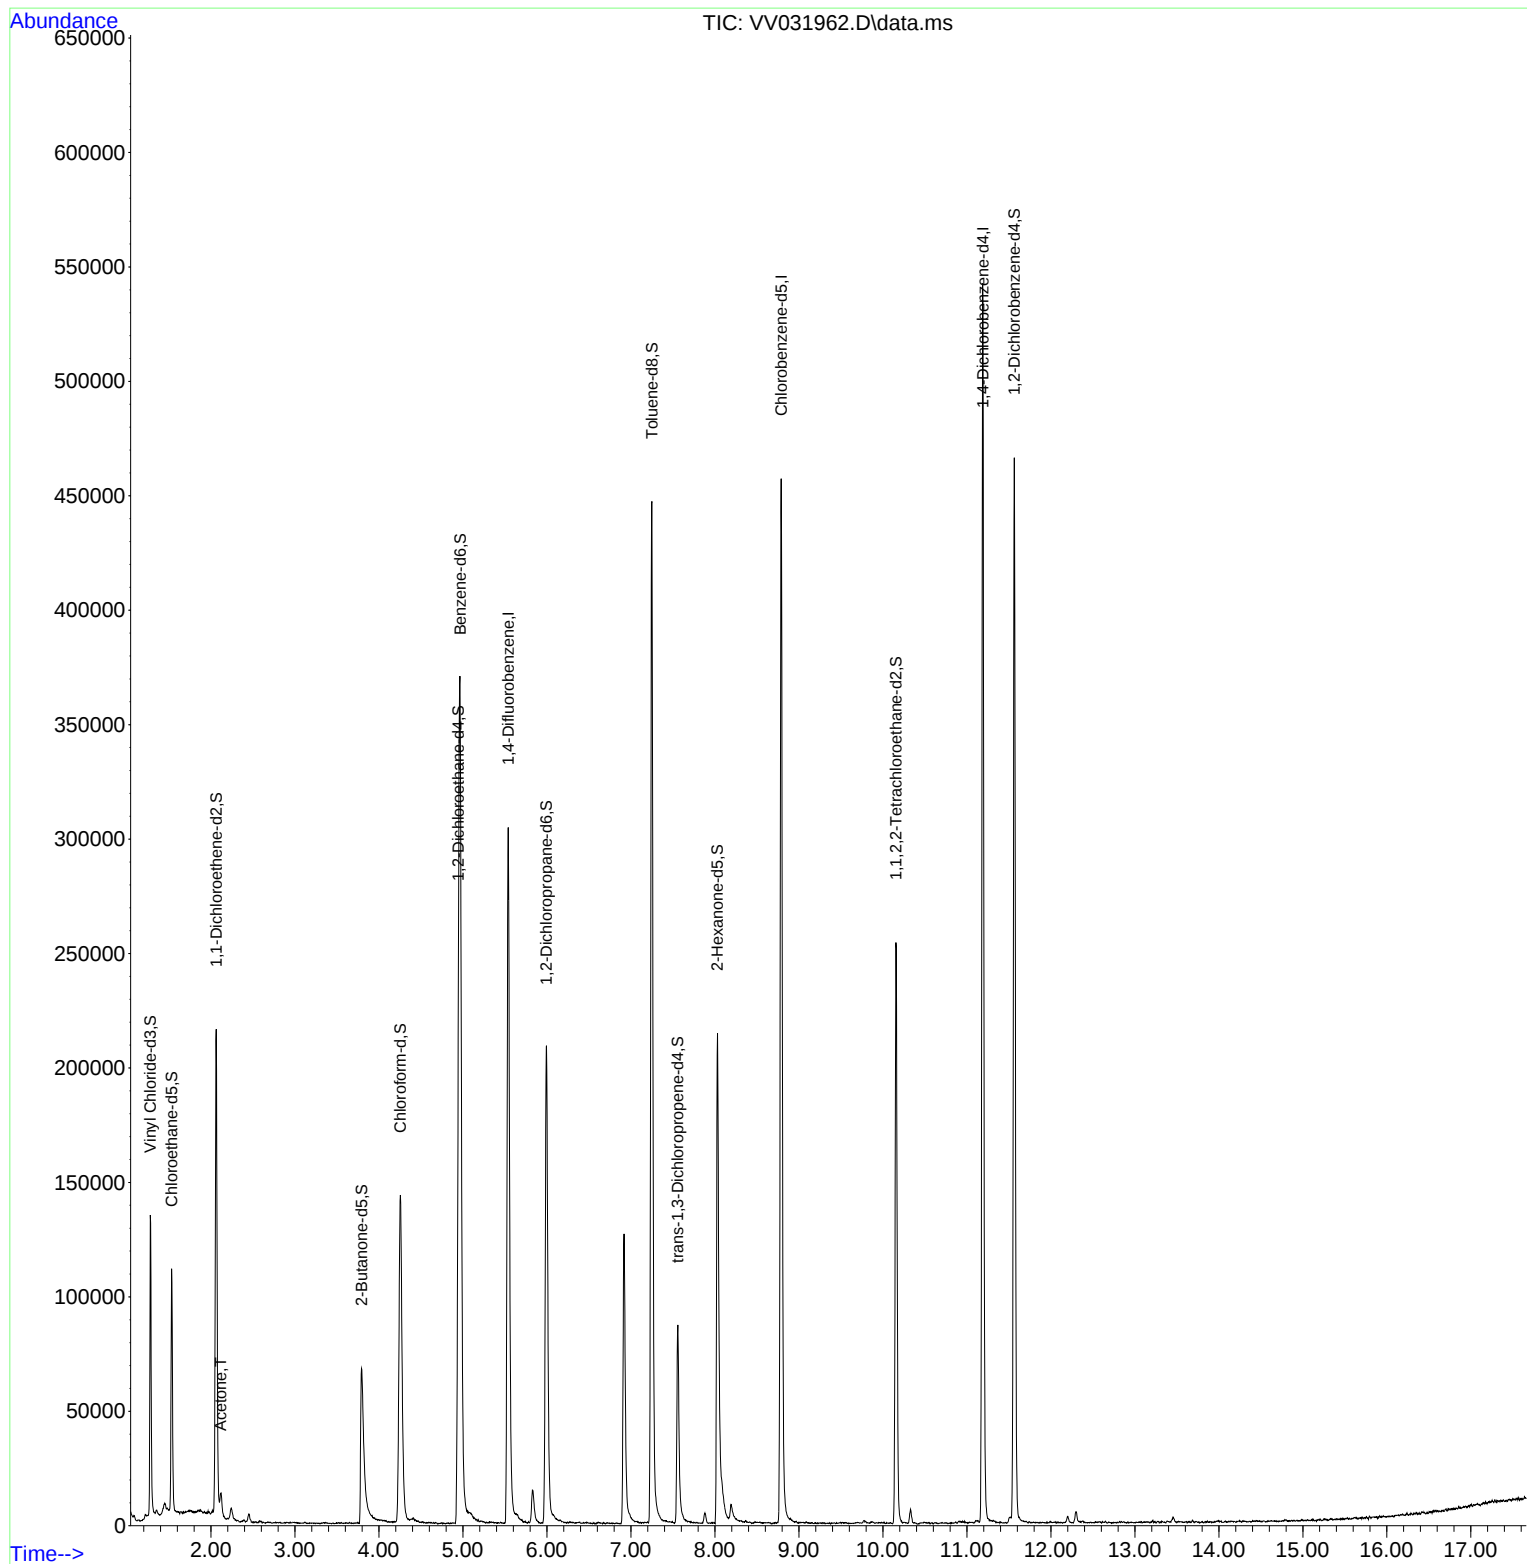

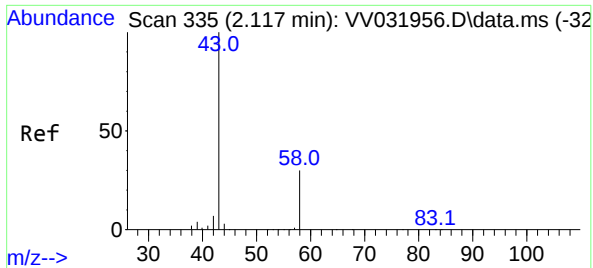

#13
 Acetone
 Concen: 7.319 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV031962.D
 Acq: 31 Aug 2023 15:31

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR5

Tgt Ion: 43 Resp: 8241
 Ion Ratio Lower Upper
 43 100
 58 36.3 0.0 61.0

