

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031957.D
 Acq On : 31 Aug 2023 13:27
 Operator : SY/MD
 Sample : VV0831MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK385

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	136659	144980	14.47%	1.831%
2	1.532	147	153	169	rVB	113057	132344	13.20%	1.671%
3	2.059	309	317	333	rVB	213618	313221	31.25%	3.955%
4	2.452	430	439	450	rBV3	7394	13071	1.30%	0.165%
5	3.121	645	647	652	rVB5	706	573	0.06%	0.007%
6	3.265	683	692	693	rBV4	456	631	0.06%	0.008%
7	3.355	717	720	722	rBV2	381	250	0.02%	0.003%
8	3.449	741	749	750	rBV2	464	549	0.05%	0.007%
9	3.606	794	798	799	rBV3	282	162	0.02%	0.002%
10	3.799	847	858	895	rBV2	77292	246324	24.58%	3.110%
11	4.252	982	999	1030	rBV	142952	376193	37.54%	4.750%
12	4.706	1139	1140	1143	rBV3	409	183	0.02%	0.002%
13	4.741	1148	1151	1152	rBV	355	197	0.02%	0.002%
14	4.831	1176	1179	1180	rBV3	448	266	0.03%	0.003%
15	4.873	1190	1192	1194	rBV2	531	234	0.02%	0.003%
16	4.960	1199	1219	1247	rBV2	377036	1002233	100.00%	12.655%
17	5.423	1361	1363	1367	rBV4	489	376	0.04%	0.005%
18	5.535	1386	1398	1423	rBV	292207	604896	60.35%	7.638%
19	5.828	1478	1489	1511	rBV3	12229	28381	2.83%	0.358%
20	5.992	1523	1540	1567	rBV	215978	458427	45.74%	5.789%
21	6.358	1653	1654	1656	rBV2	353	127	0.01%	0.002%
22	6.484	1691	1693	1695	rBV	438	271	0.03%	0.003%
23	6.522	1703	1705	1708	rVB	383	153	0.02%	0.002%
24	6.535	1708	1709	1711	rBV	221	78	0.01%	0.001%
25	6.548	1711	1713	1716	rVB3	402	177	0.02%	0.002%
26	6.561	1716	1717	1719	rVB	335	109	0.01%	0.001%
27	6.583	1722	1724	1726	rBV	345	168	0.02%	0.002%
28	6.632	1735	1739	1741	rVV4	357	221	0.02%	0.003%
29	6.645	1741	1743	1748	rVB5	714	591	0.06%	0.007%
30	6.670	1748	1751	1754	rBV2	492	386	0.04%	0.005%
31	6.854	1805	1808	1809	rBV2	533	215	0.02%	0.003%
32	6.915	1814	1827	1847	rBV	130878	247387	24.68%	3.124%
33	7.246	1919	1930	1965	rBV	462346	828835	82.70%	10.466%
34	7.554	2017	2026	2058	rBV	91294	166584	16.62%	2.103%
35	7.828	2108	2111	2115	rBV2	814	658	0.07%	0.008%
36	7.866	2121	2123	2126	rBV3	487	341	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031957.D
 Acq On : 31 Aug 2023 13:27
 Operator : SY/MD
 Sample : VV0831MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK385

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.918	2133	2139	2141	rBV3	949	694	0.07%	0.009%
38	7.976	2151	2157	2158	rBV3	414	421	0.04%	0.005%
39	8.030	2164	2174	2212	rBV	226343	447117	44.61%	5.646%
40	8.535	2329	2331	2334	rBV3	413	254	0.03%	0.003%
41	8.583	2341	2346	2350	rVB5	606	540	0.05%	0.007%
42	8.661	2365	2370	2373	rBV4	420	482	0.05%	0.006%
43	8.725	2388	2390	2392	rVB2	397	148	0.01%	0.002%
44	8.744	2393	2396	2398	rBV4	435	237	0.02%	0.003%
45	8.786	2398	2409	2437	rBV	445759	752873	75.12%	9.507%
46	9.069	2491	2497	2498	rBV2	862	651	0.06%	0.008%
47	9.242	2548	2551	2553	rBV	515	303	0.03%	0.004%
48	9.268	2557	2559	2563	rVV3	496	379	0.04%	0.005%
49	9.287	2563	2565	2568	rVB2	342	200	0.02%	0.003%
50	9.487	2616	2627	2628	rBV4	2041	2270	0.23%	0.029%
51	9.606	2662	2664	2668	rVB2	402	273	0.03%	0.003%
52	9.644	2674	2676	2677	rBV	455	236	0.02%	0.003%
53	9.667	2682	2683	2686	rBV2	422	208	0.02%	0.003%
54	9.767	2711	2714	2718	rVB5	493	310	0.03%	0.004%
55	9.786	2718	2720	2722	rBV2	188	102	0.01%	0.001%
56	9.799	2722	2724	2726	rBV2	339	165	0.02%	0.002%
57	9.876	2740	2748	2757	rBV5	2386	4219	0.42%	0.053%
58	10.104	2817	2819	2824	rBV4	425	377	0.04%	0.005%
59	10.156	2824	2835	2858	rVV	267502	428934	42.80%	5.416%
60	10.403	2909	2912	2916	rBV4	597	466	0.05%	0.006%
61	10.570	2961	2964	2966	rBV3	505	300	0.03%	0.004%
62	10.590	2966	2970	2971	rBV2	529	347	0.03%	0.004%
63	10.705	3005	3006	3007	rBV2	422	150	0.01%	0.002%
64	10.767	3023	3025	3029	rVB4	624	295	0.03%	0.004%
65	10.985	3091	3093	3096	rBV3	434	300	0.03%	0.004%
66	11.130	3132	3138	3145	rBV4	2367	3197	0.32%	0.040%
67	11.188	3145	3156	3177	rBV	517387	818453	81.66%	10.335%
68	11.448	3234	3237	3240	rBV4	459	373	0.04%	0.005%
69	11.500	3251	3253	3255	rBV	370	164	0.02%	0.002%
70	11.516	3256	3258	3261	rBV2	571	297	0.03%	0.004%
71	11.564	3261	3273	3290	rBV	481813	755737	75.41%	9.543%
72	11.898	3375	3377	3378	rBV	576	260	0.03%	0.003%
73	12.294	3499	3500	3501	rBV	252	56	0.01%	0.001%
74	12.332	3511	3512	3517	rBV4	459	321	0.03%	0.004%
75	12.593	3585	3593	3601	rBV6	5512	8362	0.83%	0.106%
76	12.828	3664	3666	3667	rBV	768	392	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031957.D
Acq On : 31 Aug 2023 13:27
Operator : SY/MD
Sample : VV0831MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK385

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

77	12.969	3706	3710	3713	rBV4	569	436	0.04%	0.006%
78	13.207	3776	3784	3793	rBV3	9888	15565	1.55%	0.197%
79	13.445	3848	3858	3877	rBV	48262	81582	8.14%	1.030%
80	13.686	3925	3933	3944	rVB3	14004	21236	2.12%	0.268%




Sum of corrected areas: 7919474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031957.D
Acq On : 31 Aug 2023 13:27
Operator : SY/MD
Sample : VV0831MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK385

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

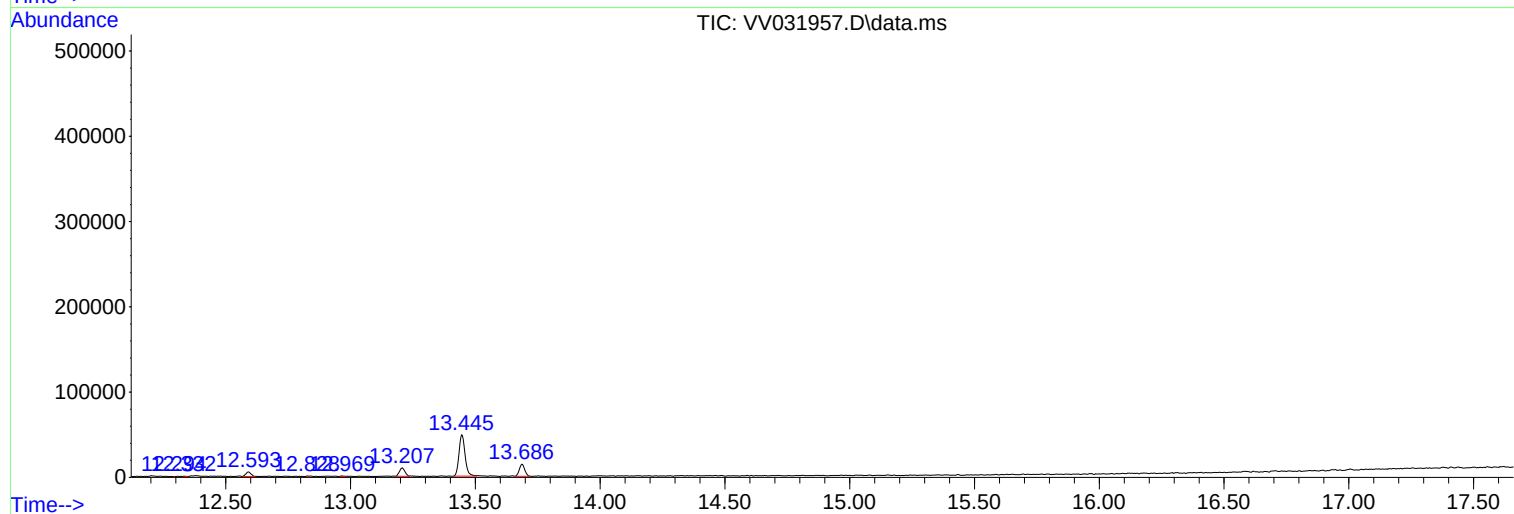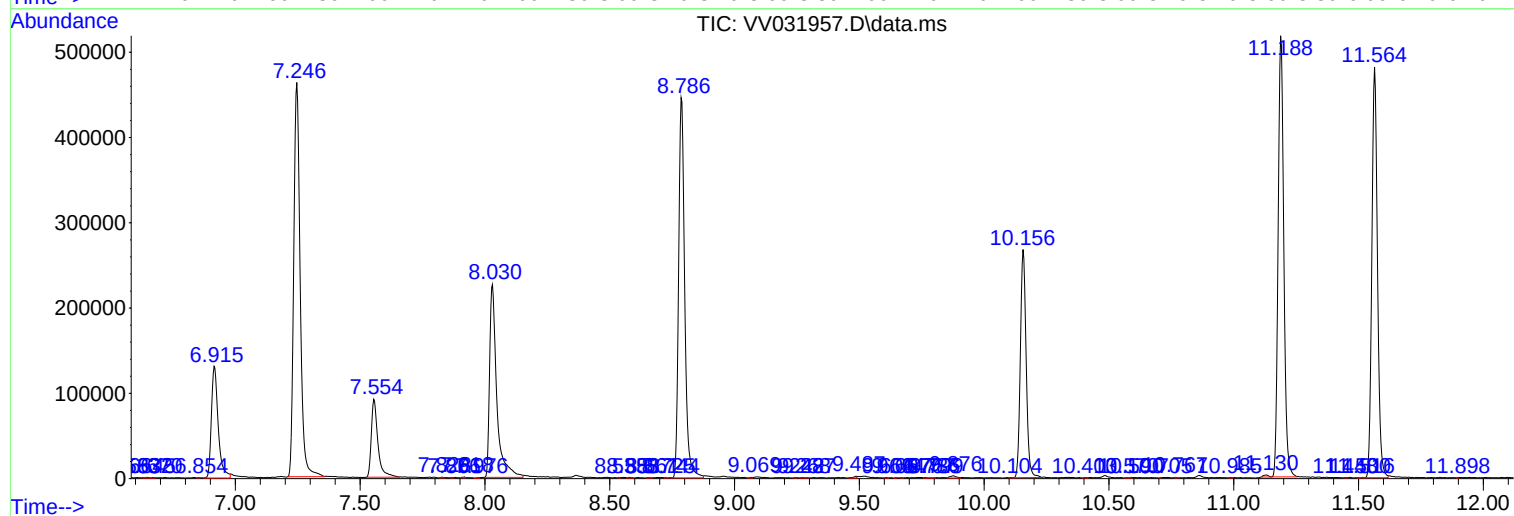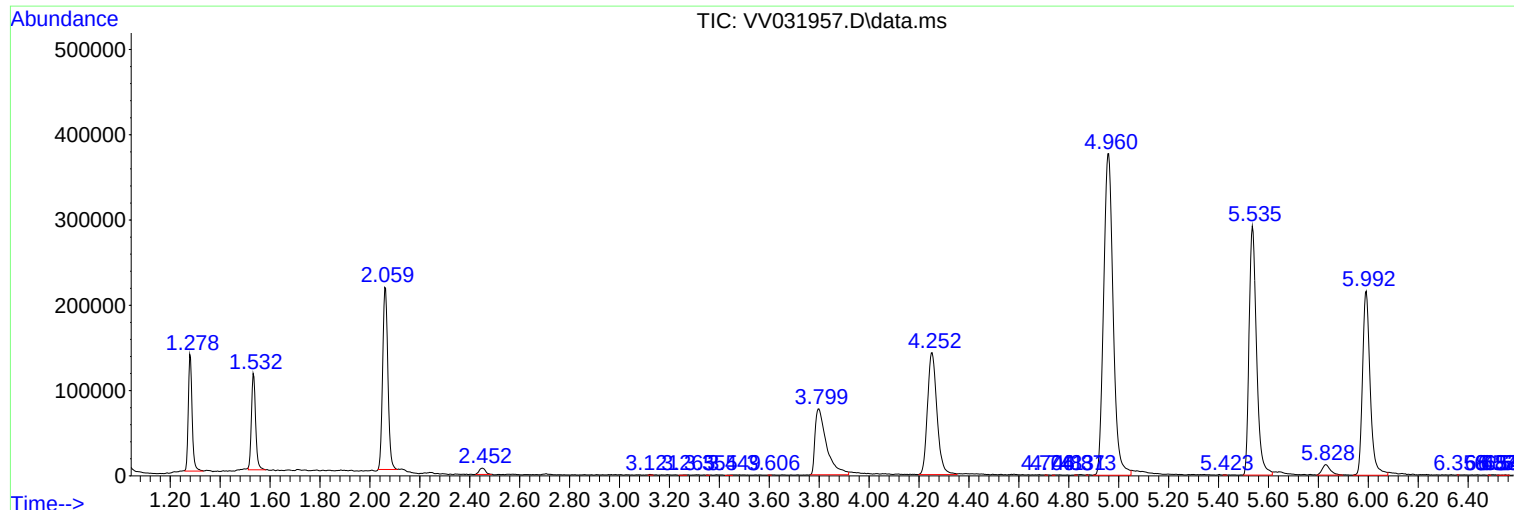

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031957.D
Acq On : 31 Aug 2023 13:27
Operator : SY/MD
Sample : VV0831MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK385

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031957.D
Acq On : 31 Aug 2023 13:27
Operator : SY/MD
Sample : VV0831MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK385

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
