

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031961.D
 Acq On : 31 Aug 2023 15:09
 Operator : SY/MD
 Sample : 04175-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rVB	132162	140070	14.49%	1.882%
2	1.532	147	153	172	rVB	108872	130152	13.46%	1.749%
3	2.063	309	318	330	rBV	207164	296057	30.62%	3.977%
4	2.828	554	556	557	rBV	243	110	0.01%	0.001%
5	2.934	587	589	591	rBV2	199	91	0.01%	0.001%
6	3.059	627	628	629	rBV	229	48	0.00%	0.001%
7	3.227	676	680	682	rBV2	424	293	0.03%	0.004%
8	3.317	705	708	711	rBV2	671	459	0.05%	0.006%
9	3.368	722	724	725	rBV	343	143	0.01%	0.002%
10	3.407	734	736	738	rBV4	340	184	0.02%	0.002%
11	3.484	758	760	764	rVB3	359	207	0.02%	0.003%
12	3.551	779	781	784	rBV	307	182	0.02%	0.002%
13	3.706	825	829	832	rBV3	562	441	0.05%	0.006%
14	3.796	847	857	895	rBV	67151	196834	20.36%	2.644%
15	4.256	985	1000	1029	rBV	138598	356402	36.87%	4.788%
16	4.555	1092	1093	1096	rBV2	383	239	0.02%	0.003%
17	4.661	1123	1126	1129	rBV2	456	352	0.04%	0.005%
18	4.709	1138	1141	1144	rBV2	435	319	0.03%	0.004%
19	4.728	1145	1147	1149	rBV2	348	175	0.02%	0.002%
20	4.776	1158	1162	1165	rBV3	245	192	0.02%	0.003%
21	4.812	1170	1173	1175	rBV	349	211	0.02%	0.003%
22	4.960	1203	1219	1246	rBV2	366679	966776	100.00%	12.988%
23	5.397	1347	1355	1356	rBV4	595	689	0.07%	0.009%
24	5.445	1365	1370	1372	rBV3	555	370	0.04%	0.005%
25	5.455	1372	1373	1375	rVV2	223	99	0.01%	0.001%
26	5.468	1375	1377	1380	rVV4	440	319	0.03%	0.004%
27	5.538	1387	1399	1419	rBV	286109	588068	60.83%	7.900%
28	5.831	1479	1490	1512	rVB4	11209	25918	2.68%	0.348%
29	5.928	1517	1520	1522	rVB3	397	174	0.02%	0.002%
30	5.940	1522	1524	1525	rBV3	177	68	0.01%	0.001%
31	5.992	1525	1540	1571	rBV	208671	441211	45.64%	5.927%
32	6.419	1671	1673	1677	rBB4	666	394	0.04%	0.005%
33	6.439	1677	1679	1680	rBV2	237	87	0.01%	0.001%
34	6.503	1697	1699	1700	rBV	382	169	0.02%	0.002%
35	6.554	1714	1715	1717	rBV	247	117	0.01%	0.002%
36	6.625	1735	1737	1740	rBV2	544	381	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031961.D
 Acq On : 31 Aug 2023 15:09
 Operator : SY/MD
 Sample : 04175-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.715	1761	1765	1768	rBV3	423	383	0.04%	0.005%
38	6.763	1775	1780	1781	rBV	331	274	0.03%	0.004%
39	6.805	1790	1793	1795	rBV2	587	330	0.03%	0.004%
40	6.831	1799	1801	1802	rBV	236	88	0.01%	0.001%
41	6.870	1807	1813	1817	rBV3	426	408	0.04%	0.005%
42	6.918	1817	1828	1859	rBV	124191	240493	24.88%	3.231%
43	7.246	1919	1930	1969	rBV	445667	802271	82.98%	10.778%
44	7.558	2017	2027	2059	rBV	84077	155733	16.11%	2.092%
45	7.831	2109	2112	2114	rBV3	378	306	0.03%	0.004%
46	7.966	2151	2154	2157	rBV3	329	220	0.02%	0.003%
47	7.979	2157	2158	2161	rVB	482	124	0.01%	0.002%
48	8.030	2165	2174	2212	rBV	208809	413699	42.79%	5.558%
49	8.516	2322	2325	2327	rBV4	541	340	0.04%	0.005%
50	8.699	2378	2382	2384	rBV2	582	499	0.05%	0.007%
51	8.728	2387	2391	2392	rBV3	420	296	0.03%	0.004%
52	8.789	2398	2410	2435	rBV	438815	733882	75.91%	9.859%
53	9.037	2484	2487	2491	rBV3	494	394	0.04%	0.005%
54	9.265	2553	2558	2563	rBV4	511	588	0.06%	0.008%
55	9.358	2584	2587	2590	rVB2	466	251	0.03%	0.003%
56	9.374	2590	2592	2595	rBV3	254	172	0.02%	0.002%
57	9.390	2595	2597	2600	rBV	281	153	0.02%	0.002%
58	9.458	2616	2618	2620	rVB2	368	122	0.01%	0.002%
59	9.558	2646	2649	2651	rBV2	293	231	0.02%	0.003%
60	9.641	2673	2675	2680	rVB2	667	481	0.05%	0.006%
61	9.667	2680	2683	2685	rBV3	503	381	0.04%	0.005%
62	9.696	2690	2692	2696	rVV3	739	484	0.05%	0.007%
63	9.731	2700	2703	2706	rBV3	462	342	0.04%	0.005%
64	9.879	2747	2749	2752	rVB3	492	218	0.02%	0.003%
65	10.017	2789	2792	2795	rBV3	465	340	0.04%	0.005%
66	10.088	2808	2814	2815	rBV3	619	516	0.05%	0.007%
67	10.156	2824	2835	2857	rBV	254439	412845	42.70%	5.546%
68	10.281	2872	2874	2878	rBV2	420	261	0.03%	0.004%
69	10.329	2878	2889	2902	rVV4	8416	14213	1.47%	0.191%
70	10.439	2921	2923	2924	rBV	373	185	0.02%	0.002%
71	10.519	2945	2948	2949	rBV2	301	163	0.02%	0.002%
72	10.686	2998	3000	3002	rBV	277	151	0.02%	0.002%
73	10.728	3010	3013	3015	rBV3	427	265	0.03%	0.004%
74	10.744	3015	3018	3021	rBV	403	330	0.03%	0.004%
75	10.776	3025	3028	3029	rBV	361	217	0.02%	0.003%
76	10.799	3033	3035	3037	rBV	397	152	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031961.D
 Acq On : 31 Aug 2023 15:09
 Operator : SY/MD
 Sample : 04175-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

77	10.918	3066	3072	3073	rBV3	746	757	0.08%	0.010%
78	11.188	3145	3156	3184	rBV	503854	791337	81.85%	10.631%
79	11.464	3240	3242	3243	rBV	292	111	0.01%	0.001%
80	11.564	3262	3273	3294	rVB	448216	705738	73.00%	9.481%
81	11.992	3401	3406	3412	rBV4	689	723	0.07%	0.010%
82	12.297	3492	3501	3511	rBV7	6807	12501	1.29%	0.168%
83	12.802	3656	3658	3662	rBV4	500	396	0.04%	0.005%
84	13.631	3914	3916	3921	rVB3	1093	854	0.09%	0.011%
85	13.657	3921	3924	3925	rBV	745	396	0.04%	0.005%




Sum of corrected areas: 7443615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031961.D
Acq On : 31 Aug 2023 15:09
Operator : SY/MD
Sample : 04175-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYPO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

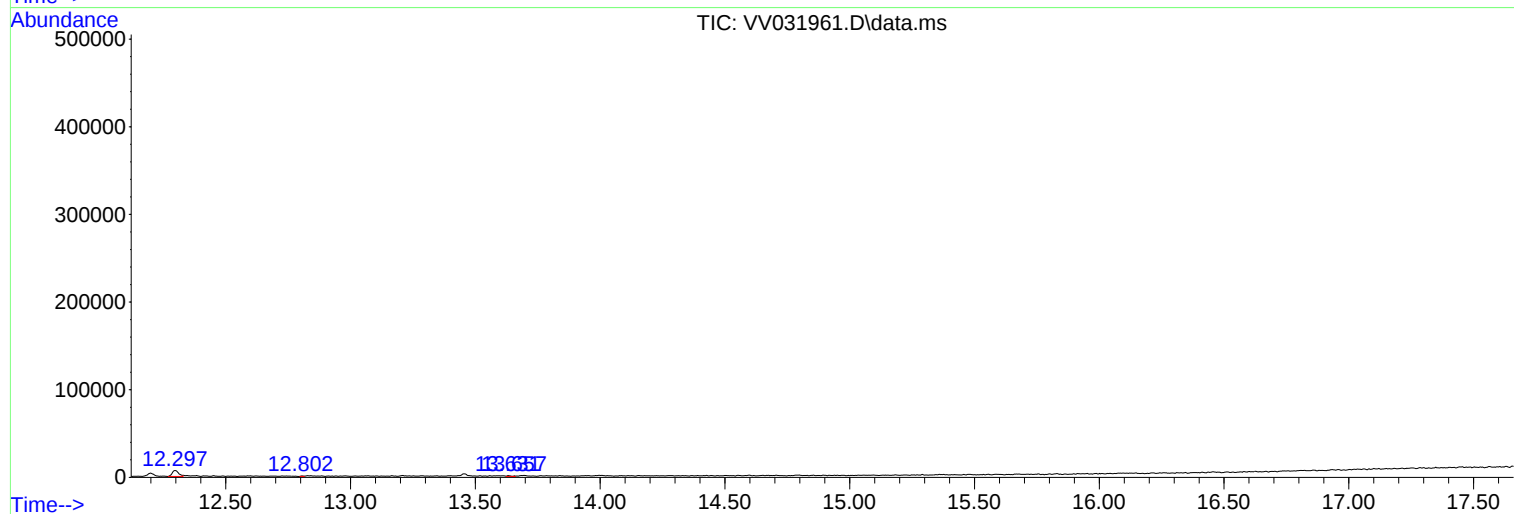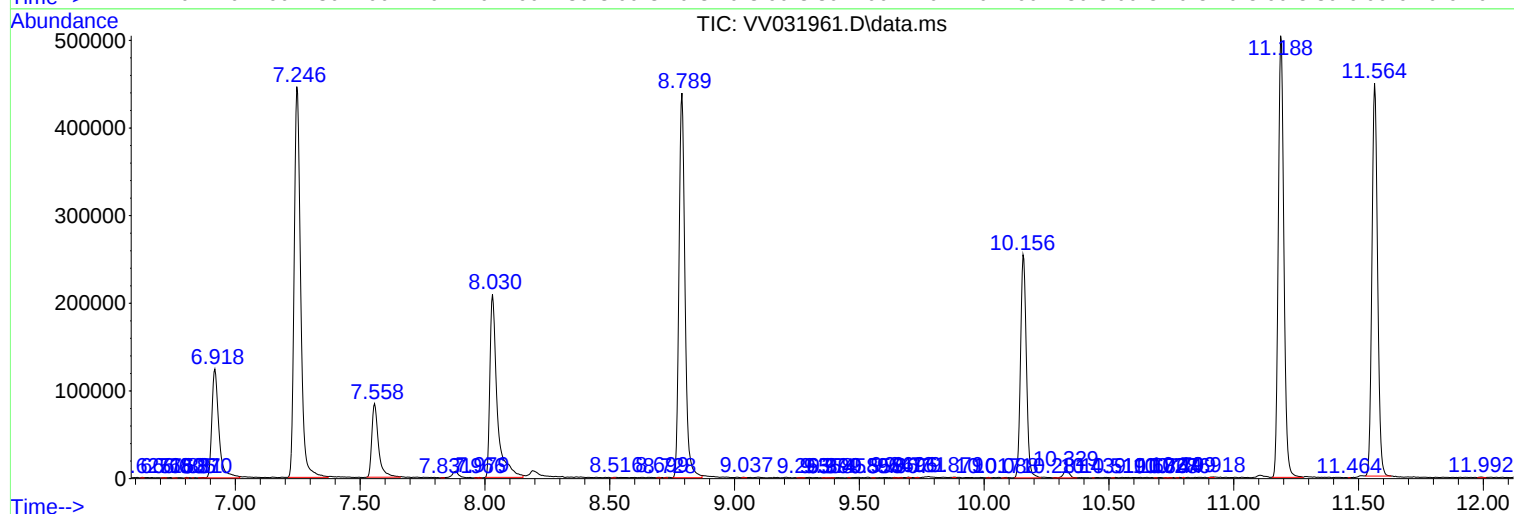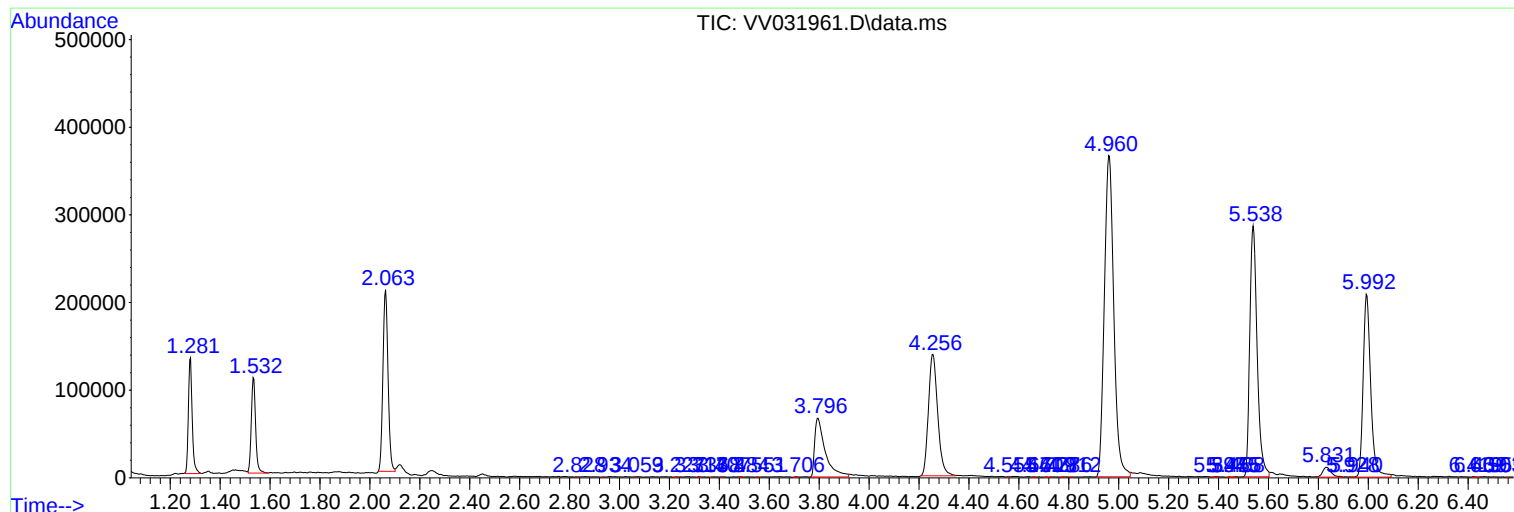

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031961.D
Acq On : 31 Aug 2023 15:09
Operator : SY/MD
Sample : 04175-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031961.D
Acq On : 31 Aug 2023 15:09
Operator : SY/MD
Sample : 04175-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYPO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc