

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031963.D
 Acq On : 31 Aug 2023 15:55
 Operator : SY/MD
 Sample : 04235-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	129280	137861	14.29%	1.790%
2	1.532	147	153	168	rVB	106492	124818	12.94%	1.620%
3	2.063	309	318	330	rBV	201475	290457	30.11%	3.771%
4	2.892	574	576	583	rVB4	664	415	0.04%	0.005%
5	3.108	640	643	646	rBV3	439	335	0.03%	0.004%
6	3.175	661	664	666	rBV3	362	305	0.03%	0.004%
7	3.291	698	700	704	rVB3	278	217	0.02%	0.003%
8	3.327	708	711	716	rVB4	630	494	0.05%	0.006%
9	3.372	723	725	730	rBV3	503	319	0.03%	0.004%
10	3.394	730	732	735	rVB2	349	164	0.02%	0.002%
11	3.410	735	737	739	rBV	383	225	0.02%	0.003%
12	3.423	739	741	744	rVV3	523	331	0.03%	0.004%
13	3.445	747	748	750	rBV2	361	125	0.01%	0.002%
14	3.468	754	755	758	rBV	322	152	0.02%	0.002%
15	3.497	758	764	770	rVB4	528	601	0.06%	0.008%
16	3.642	807	809	812	rBV3	288	172	0.02%	0.002%
17	3.748	840	842	844	rBV2	458	303	0.03%	0.004%
18	3.796	848	857	893	rBV	66630	193407	20.05%	2.511%
19	4.256	985	1000	1034	rBV	138788	358822	37.19%	4.658%
20	4.667	1127	1128	1130	rBV	314	126	0.01%	0.002%
21	4.867	1188	1190	1192	rVB2	405	172	0.02%	0.002%
22	4.960	1199	1219	1254	rBV2	364205	964746	100.00%	12.525%
23	5.371	1343	1347	1349	rBV	369	304	0.03%	0.004%
24	5.381	1349	1350	1355	rVV3	441	250	0.03%	0.003%
25	5.445	1369	1370	1375	rBV2	282	201	0.02%	0.003%
26	5.484	1380	1382	1386	rBV2	383	328	0.03%	0.004%
27	5.539	1387	1399	1425	rBV	320481	658979	68.31%	8.555%
28	5.828	1479	1489	1508	rBV2	14595	32689	3.39%	0.424%
29	5.928	1517	1520	1522	rBV2	486	327	0.03%	0.004%
30	5.992	1526	1540	1562	rBV	205259	433035	44.89%	5.622%
31	6.378	1656	1660	1661	rBV2	449	320	0.03%	0.004%
32	6.487	1692	1694	1700	rBV3	347	348	0.04%	0.005%
33	6.532	1706	1708	1711	rVB	314	131	0.01%	0.002%
34	6.568	1715	1719	1720	rBV2	598	315	0.03%	0.004%
35	6.580	1720	1723	1724	rBV	447	204	0.02%	0.003%
36	6.632	1737	1739	1740	rBV2	397	208	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031963.D
 Acq On : 31 Aug 2023 15:55
 Operator : SY/MD
 Sample : 04235-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.674	1751	1752	1755	rBV2	233	144	0.01%	0.002%
38	6.741	1770	1773	1774	rVV2	321	181	0.02%	0.002%
39	6.799	1788	1791	1794	rBV2	461	351	0.04%	0.005%
40	6.828	1797	1800	1803	rVB2	381	264	0.03%	0.003%
41	6.873	1810	1814	1816	rBV2	345	288	0.03%	0.004%
42	6.918	1817	1828	1858	rVV	122749	237137	24.58%	3.079%
43	7.246	1919	1930	1974	rBV	440095	796150	82.52%	10.336%
44	7.558	2017	2027	2050	rBV	85220	157834	16.36%	2.049%
45	7.828	2109	2111	2112	rBV2	397	149	0.02%	0.002%
46	7.879	2120	2127	2136	rBV2	2490	4439	0.46%	0.058%
47	7.976	2152	2157	2161	rBV4	699	683	0.07%	0.009%
48	8.030	2163	2174	2211	rBV	217392	430837	44.66%	5.593%
49	8.445	2300	2303	2304	rBV3	513	246	0.03%	0.003%
50	8.593	2346	2349	2350	rBV3	663	447	0.05%	0.006%
51	8.664	2369	2371	2374	rVB2	451	193	0.02%	0.003%
52	8.683	2374	2377	2379	rBV	472	280	0.03%	0.004%
53	8.696	2379	2381	2382	rBV2	437	190	0.02%	0.002%
54	8.789	2398	2410	2439	rBV	492956	826139	85.63%	10.725%
55	9.063	2493	2495	2497	rBV3	399	285	0.03%	0.004%
56	9.169	2526	2528	2530	rVB2	339	152	0.02%	0.002%
57	9.182	2530	2532	2534	rBV2	673	340	0.04%	0.004%
58	9.217	2540	2543	2545	rVB3	463	197	0.02%	0.003%
59	9.259	2553	2556	2559	rBV	363	269	0.03%	0.003%
60	9.288	2561	2565	2568	rBV3	461	348	0.04%	0.005%
61	9.326	2575	2577	2579	rBV3	277	156	0.02%	0.002%
62	9.339	2579	2581	2584	rVB2	458	210	0.02%	0.003%
63	9.400	2596	2600	2602	rVB2	403	281	0.03%	0.004%
64	9.497	2620	2630	2633	rBV5	1642	2395	0.25%	0.031%
65	9.747	2705	2708	2710	rBV2	412	310	0.03%	0.004%
66	9.870	2741	2746	2748	rBV3	1358	1326	0.14%	0.017%
67	10.046	2797	2801	2803	rBV2	640	460	0.05%	0.006%
68	10.111	2818	2821	2823	rBV	558	302	0.03%	0.004%
69	10.156	2823	2835	2851	rBV	248929	403115	41.78%	5.233%
70	10.301	2876	2880	2881	rBV2	367	242	0.03%	0.003%
71	10.329	2882	2889	2898	rVB5	4152	6540	0.68%	0.085%
72	10.400	2904	2911	2915	rVB4	480	634	0.07%	0.008%
73	10.429	2915	2920	2922	rBV	589	487	0.05%	0.006%
74	10.487	2930	2938	2946	rBV4	1361	2297	0.24%	0.030%
75	10.638	2980	2985	2987	rBV2	314	225	0.02%	0.003%
76	10.673	2992	2996	2997	rBV2	441	294	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031963.D
 Acq On : 31 Aug 2023 15:55
 Operator : SY/MD
 Sample : 04235-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.693	3000	3002	3006	rVB3	627	308	0.03%	0.004%
78	10.712	3006	3008	3012	rVB	454	211	0.02%	0.003%
79	10.738	3012	3016	3017	rBV2	302	195	0.02%	0.003%
80	10.783	3026	3030	3032	rBV3	557	379	0.04%	0.005%
81	10.796	3032	3034	3037	rVV3	359	228	0.02%	0.003%
82	10.863	3049	3055	3061	rBV5	1334	1641	0.17%	0.021%
83	10.892	3061	3064	3066	rBV4	812	673	0.07%	0.009%
84	11.188	3145	3156	3186	rBV	562002	887282	91.97%	11.519%
85	11.410	3224	3225	3228	rBV3	381	186	0.02%	0.002%
86	11.464	3239	3242	3245	rBV2	420	287	0.03%	0.004%
87	11.509	3247	3256	3261	rVV6	3582	6355	0.66%	0.083%
88	11.564	3263	3273	3294	rVB	448407	710687	73.67%	9.227%
89	11.731	3324	3325	3327	rBV	430	188	0.02%	0.002%
90	12.169	3458	3461	3462	rBV	625	366	0.04%	0.005%
91	12.297	3494	3501	3511	rBV7	5755	9389	0.97%	0.122%
92	12.657	3610	3613	3616	rBV4	530	438	0.05%	0.006%
93	12.799	3654	3657	3659	rBV3	539	340	0.04%	0.004%
94	12.988	3711	3716	3717	rBV3	569	456	0.05%	0.006%
95	13.156	3766	3768	3771	rBV3	571	351	0.04%	0.005%
96	13.175	3771	3774	3775	rBV	390	230	0.02%	0.003%
97	13.210	3780	3785	3793	rVB5	1710	2153	0.22%	0.028%
98	13.246	3793	3796	3798	rBV2	535	347	0.04%	0.005%
99	13.509	3874	3878	3881	rVB3	706	500	0.05%	0.006%
100	13.660	3921	3925	3926	rBV2	494	409	0.04%	0.005%




Sum of corrected areas: 7702622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031963.D
Acq On : 31 Aug 2023 15:55
Operator : SY/MD
Sample : 04235-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

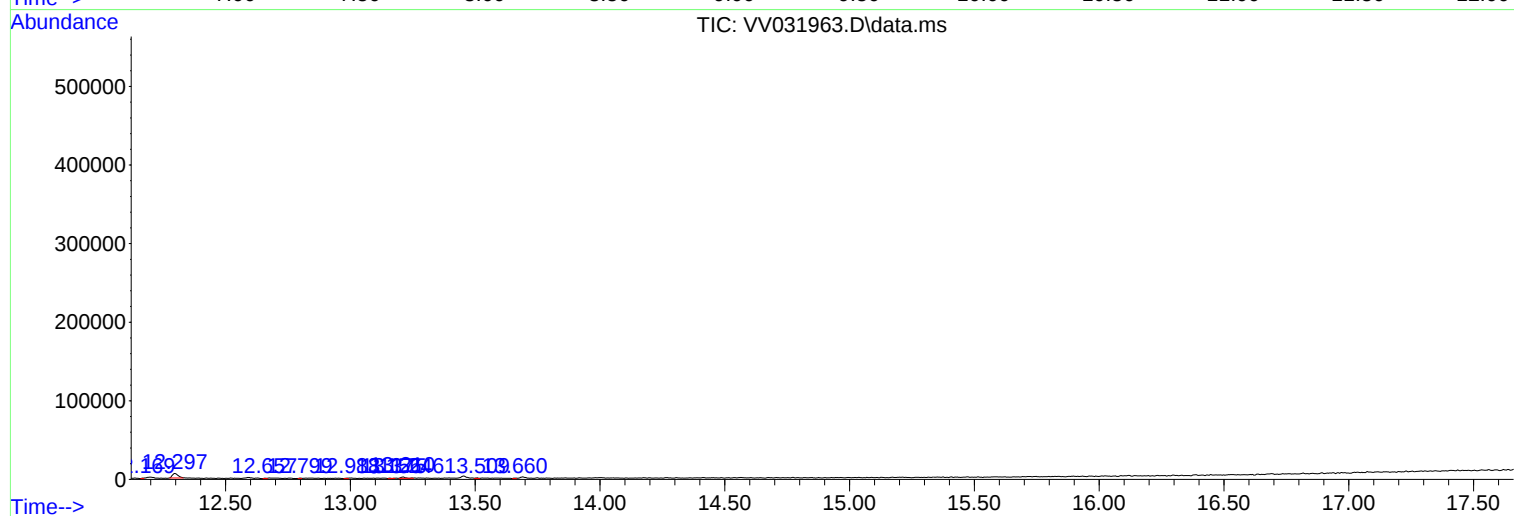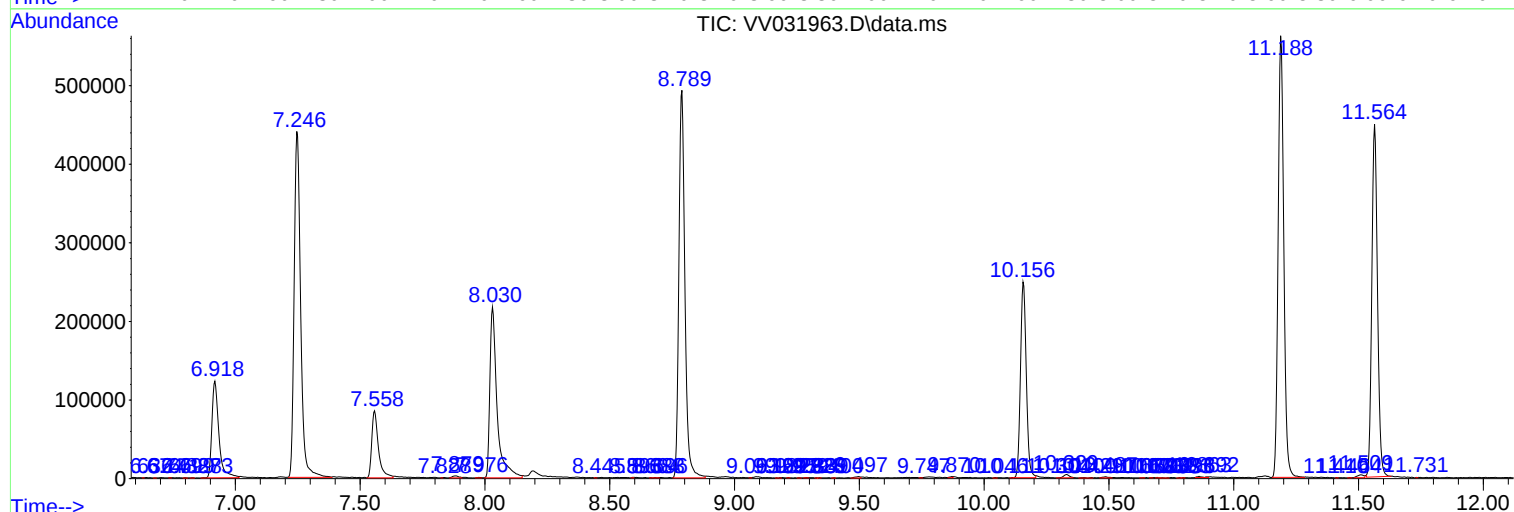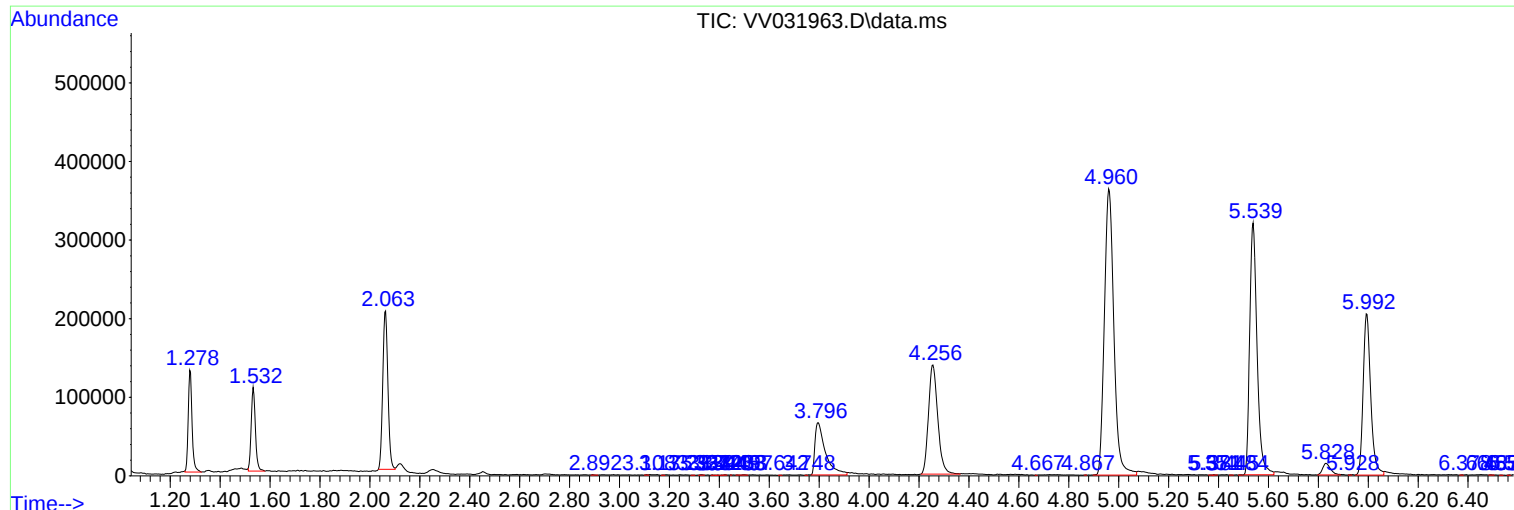

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031963.D
Acq On : 31 Aug 2023 15:55
Operator : SY/MD
Sample : 04235-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYPI

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031963.D
Acq On : 31 Aug 2023 15:55
Operator : SY/MD
Sample : 04235-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYPI

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------