

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031964.D
 Acq On : 31 Aug 2023 16:18
 Operator : SY/MD
 Sample : 04235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	128487	138280	14.33%	1.791%
2	1.532	147	153	168	rVB	107362	124751	12.92%	1.615%
3	2.063	309	318	330	rBV	202473	292698	30.32%	3.790%
4	2.745	528	530	532	rBV2	321	170	0.02%	0.002%
5	2.963	594	598	600	rBV3	609	582	0.06%	0.008%
6	3.044	620	623	627	rBV2	409	442	0.05%	0.006%
7	3.134	650	651	652	rBV2	361	131	0.01%	0.002%
8	3.172	661	663	666	rBV2	294	201	0.02%	0.003%
9	3.275	690	695	696	rBV2	399	311	0.03%	0.004%
10	3.404	731	735	737	rBV	472	321	0.03%	0.004%
11	3.436	743	745	747	rBV2	230	132	0.01%	0.002%
12	3.452	747	750	752	rVV3	538	360	0.04%	0.005%
13	3.465	752	754	758	rVV4	503	373	0.04%	0.005%
14	3.497	762	764	768	rVB2	289	186	0.02%	0.002%
15	3.565	783	785	788	rVB2	274	154	0.02%	0.002%
16	3.593	791	794	796	rBV3	794	531	0.06%	0.007%
17	3.664	815	816	821	rBV3	242	215	0.02%	0.003%
18	3.796	848	857	888	rBV	64679	184894	19.15%	2.394%
19	4.256	984	1000	1031	rBV	138183	361395	37.44%	4.680%
20	4.664	1123	1127	1128	rBV	575	392	0.04%	0.005%
21	4.703	1137	1139	1141	rBV	378	234	0.02%	0.003%
22	4.767	1153	1159	1160	rBV4	624	479	0.05%	0.006%
23	4.960	1201	1219	1251	rBV2	363873	965294	100.00%	12.499%
24	5.204	1293	1295	1299	rBV4	615	456	0.05%	0.006%
25	5.323	1329	1332	1336	rBV4	616	518	0.05%	0.007%
26	5.539	1387	1399	1427	rBV	327975	670603	69.47%	8.684%
27	5.793	1476	1478	1480	rBV4	457	249	0.03%	0.003%
28	5.831	1480	1490	1507	rVV2	14042	30752	3.19%	0.398%
29	5.934	1519	1522	1525	rVB2	276	197	0.02%	0.003%
30	5.992	1525	1540	1579	rBV	206736	446408	46.25%	5.780%
31	6.352	1649	1652	1653	rBV2	250	152	0.02%	0.002%
32	6.362	1653	1655	1659	rVV4	572	446	0.05%	0.006%
33	6.394	1663	1665	1670	rVB3	418	306	0.03%	0.004%
34	6.461	1684	1686	1688	rBV3	442	230	0.02%	0.003%
35	6.574	1718	1721	1725	rBV2	444	332	0.03%	0.004%
36	6.632	1737	1739	1743	rVB3	682	359	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031964.D
 Acq On : 31 Aug 2023 16:18
 Operator : SY/MD
 Sample : 04235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.677	1751	1753	1755	rBV2	354	158	0.02%	0.002%
38	6.728	1765	1769	1772	rBB2	265	174	0.02%	0.002%
39	6.841	1800	1804	1806	rBV2	348	331	0.03%	0.004%
40	6.918	1816	1828	1853	rBV	123972	238976	24.76%	3.094%
41	7.246	1917	1930	1963	rBV	443948	799639	82.84%	10.354%
42	7.558	2017	2027	2056	rBV2	83754	157892	16.36%	2.045%
43	7.854	2112	2119	2121	rBV4	730	692	0.07%	0.009%
44	7.876	2121	2126	2127	rBV4	1399	1171	0.12%	0.015%
45	7.979	2155	2158	2161	rBV3	302	249	0.03%	0.003%
46	8.031	2164	2174	2213	rBV	214093	423962	43.92%	5.490%
47	8.465	2307	2309	2316	rVB5	463	310	0.03%	0.004%
48	8.596	2348	2350	2352	rVB	378	208	0.02%	0.003%
49	8.613	2352	2355	2356	rBV3	289	132	0.01%	0.002%
50	8.648	2362	2366	2367	rBV3	380	248	0.03%	0.003%
51	8.712	2383	2386	2390	rVB4	635	505	0.05%	0.007%
52	8.732	2390	2392	2393	rBV4	586	237	0.02%	0.003%
53	8.741	2393	2395	2398	rVB	355	155	0.02%	0.002%
54	8.789	2398	2410	2441	rBV	495187	836459	86.65%	10.831%
55	9.082	2498	2501	2504	rVB4	597	404	0.04%	0.005%
56	9.159	2523	2525	2528	rBV2	297	202	0.02%	0.003%
57	9.220	2542	2544	2547	rVB2	327	145	0.02%	0.002%
58	9.236	2547	2549	2550	rBV2	294	145	0.02%	0.002%
59	9.326	2574	2577	2579	rVV3	283	162	0.02%	0.002%
60	9.426	2606	2608	2611	rBV2	352	270	0.03%	0.003%
61	9.461	2616	2619	2622	rBV3	435	295	0.03%	0.004%
62	9.558	2646	2649	2652	rBV3	262	172	0.02%	0.002%
63	9.577	2652	2655	2656	rBV3	307	181	0.02%	0.002%
64	9.658	2677	2680	2681	rBV2	332	190	0.02%	0.002%
65	9.770	2706	2715	2718	rBV4	862	1198	0.12%	0.016%
66	9.844	2735	2738	2740	rBV3	442	264	0.03%	0.003%
67	9.934	2762	2766	2767	rVB	463	259	0.03%	0.003%
68	10.014	2789	2791	2794	rVB2	396	262	0.03%	0.003%
69	10.034	2794	2797	2800	rBV2	383	323	0.03%	0.004%
70	10.066	2805	2807	2809	rVB	458	191	0.02%	0.002%
71	10.088	2809	2814	2818	rBV4	379	426	0.04%	0.006%
72	10.156	2824	2835	2855	rBV	252320	401079	41.55%	5.194%
73	10.284	2873	2875	2878	rBV2	412	206	0.02%	0.003%
74	10.330	2881	2889	2898	rBV3	3105	5336	0.55%	0.069%
75	10.391	2905	2908	2910	rBV4	363	280	0.03%	0.004%
76	10.432	2918	2921	2922	rBV2	515	209	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031964.D
 Acq On : 31 Aug 2023 16:18
 Operator : SY/MD
 Sample : 04235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.465	2928	2931	2933	rBV	393	250	0.03%	0.003%
78	10.519	2946	2948	2951	rVB2	348	183	0.02%	0.002%
79	10.561	2959	2961	2964	rBV	363	139	0.01%	0.002%
80	10.648	2984	2988	2992	rBV2	240	273	0.03%	0.004%
81	10.670	2992	2995	3000	rVB4	552	451	0.05%	0.006%
82	10.693	3000	3002	3005	rBV	454	261	0.03%	0.003%
83	10.744	3014	3018	3021	rBV	532	335	0.03%	0.004%
84	10.757	3021	3022	3023	rBV	367	129	0.01%	0.002%
85	10.844	3046	3049	3050	rBV	250	144	0.01%	0.002%
86	11.079	3119	3122	3124	rBV2	248	207	0.02%	0.003%
87	11.104	3124	3130	3137	rBV6	1697	2476	0.26%	0.032%
88	11.188	3145	3156	3176	rBV	582357	891581	92.36%	11.545%
89	11.403	3220	3223	3224	rBV	422	178	0.02%	0.002%
90	11.481	3243	3247	3248	rBV2	675	532	0.06%	0.007%
91	11.510	3248	3256	3261	rVV7	3171	5777	0.60%	0.075%
92	11.564	3262	3273	3291	rVB	449798	705458	73.08%	9.135%
93	11.979	3397	3402	3403	rBV2	713	595	0.06%	0.008%
94	12.194	3463	3469	3475	rBV7	1900	2327	0.24%	0.030%
95	12.297	3493	3501	3511	rBV4	7334	12951	1.34%	0.168%
96	12.641	3606	3608	3609	rBV	498	188	0.02%	0.002%
97	12.667	3613	3616	3618	rBV	424	260	0.03%	0.003%
98	13.059	3735	3738	3740	rBV3	548	285	0.03%	0.004%
99	13.140	3761	3763	3765	rBV	346	156	0.02%	0.002%
100	13.635	3915	3917	3919	rBV2	576	338	0.04%	0.004%




Sum of corrected areas: 7722705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031964.D
Acq On : 31 Aug 2023 16:18
Operator : SY/MD
Sample : 04235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

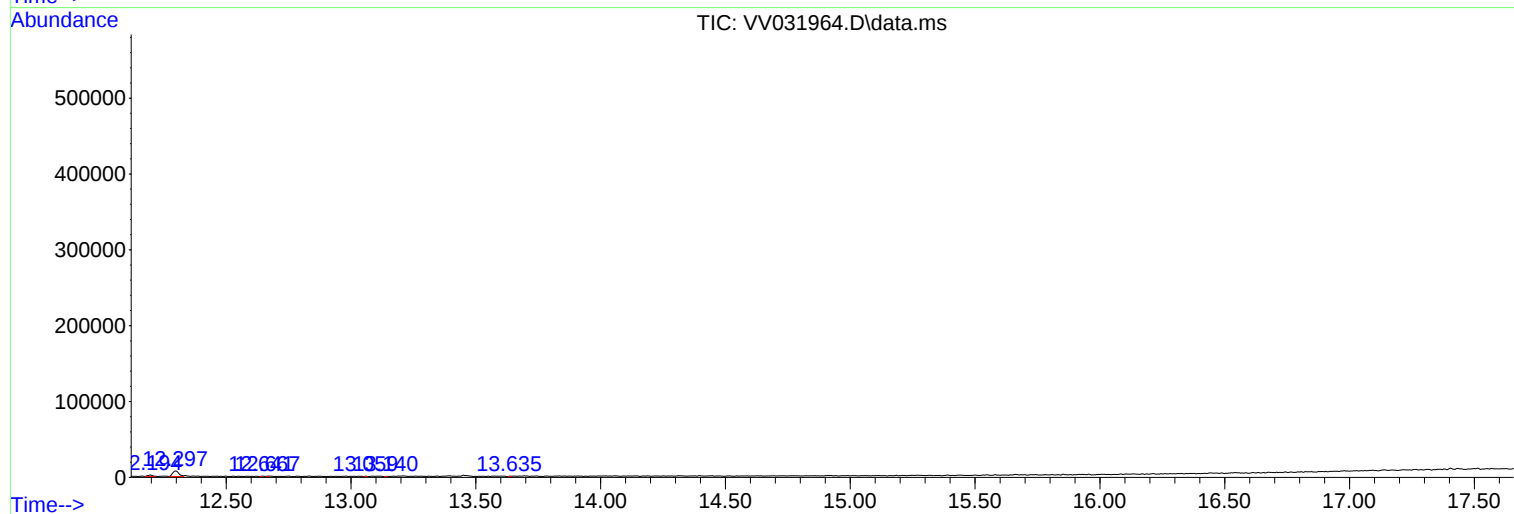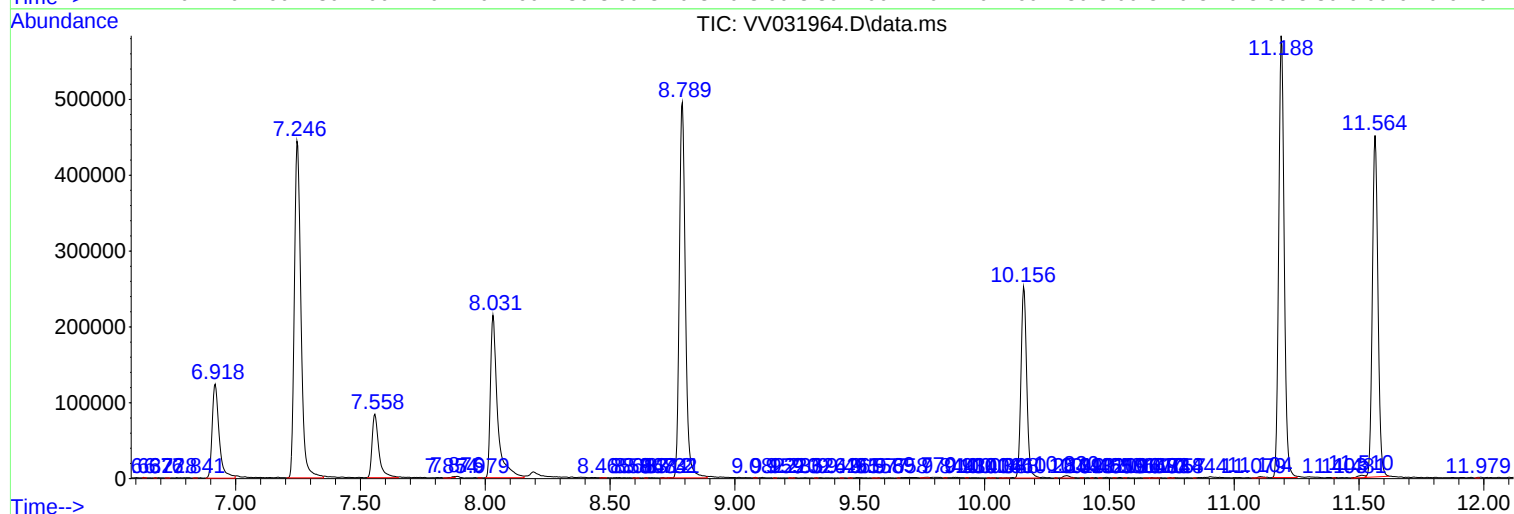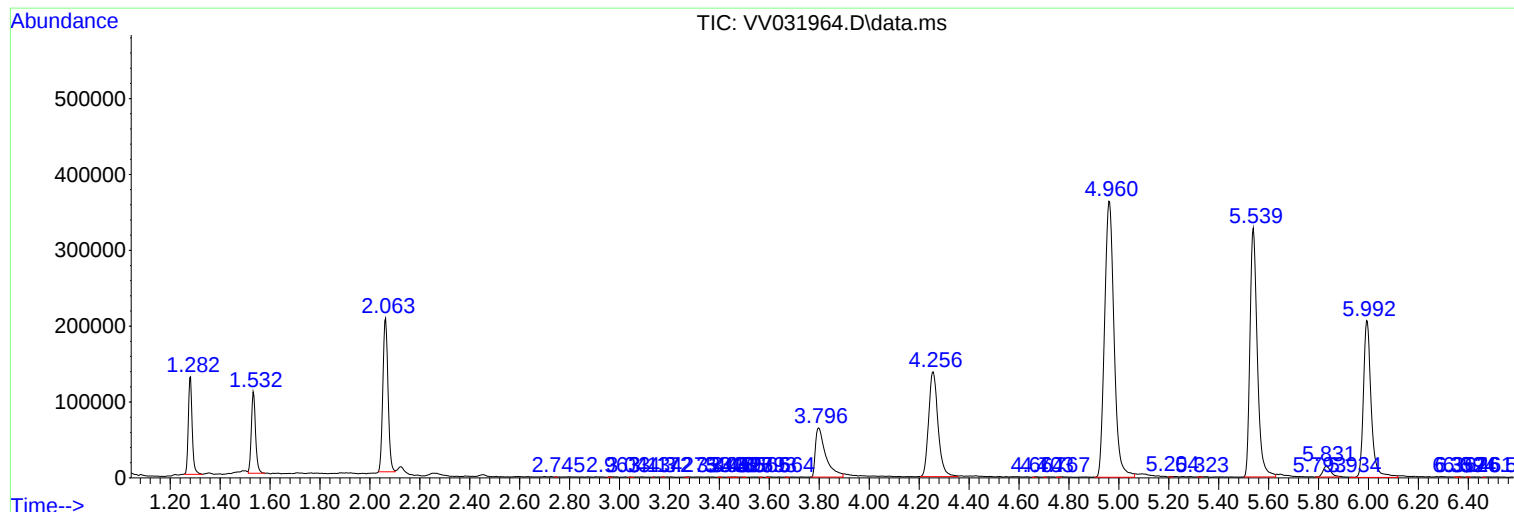

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031964.D
Acq On : 31 Aug 2023 16:18
Operator : SY/MD
Sample : 04235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031964.D
Acq On : 31 Aug 2023 16:18
Operator : SY/MD
Sample : 04235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
