

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031966.D
 Acq On : 31 Aug 2023 17:04
 Operator : SY/MD
 Sample : 04235-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	124119	129610	13.93%	1.746%
2	1.536	148	154	171	rVB	102395	118550	12.74%	1.597%
3	2.063	309	318	334	rBV	194613	282528	30.36%	3.805%
4	2.889	572	575	576	rBV	344	178	0.02%	0.002%
5	2.928	583	587	588	rBV2	275	207	0.02%	0.003%
6	3.111	639	644	645	rBV2	440	283	0.03%	0.004%
7	3.143	652	654	657	rBV4	226	170	0.02%	0.002%
8	3.256	684	689	691	rBV3	607	514	0.06%	0.007%
9	3.497	762	764	767	rVB3	343	160	0.02%	0.002%
10	3.564	783	785	787	rVB2	395	120	0.01%	0.002%
11	3.670	816	818	820	rBV	221	126	0.01%	0.002%
12	3.754	839	844	847	rBV4	530	578	0.06%	0.008%
13	3.802	850	859	888	rBV2	66347	199928	21.48%	2.693%
14	4.256	985	1000	1035	rVB	132084	339921	36.53%	4.579%
15	4.670	1127	1129	1131	rBV	300	118	0.01%	0.002%
16	4.760	1153	1157	1159	rBV2	498	303	0.03%	0.004%
17	4.802	1167	1170	1172	rVB2	364	203	0.02%	0.003%
18	4.822	1172	1176	1179	rBV3	508	419	0.05%	0.006%
19	4.963	1199	1220	1252	rBV2	350452	930572	100.00%	12.534%
20	5.249	1306	1309	1310	rBV2	633	378	0.04%	0.005%
21	5.330	1332	1334	1338	rBV	478	267	0.03%	0.004%
22	5.458	1372	1374	1377	rBV3	351	204	0.02%	0.003%
23	5.539	1383	1399	1427	rBV	310578	643728	69.18%	8.671%
24	5.831	1480	1490	1510	rBV3	9374	21050	2.26%	0.284%
25	5.995	1527	1541	1564	rBV	200006	420866	45.23%	5.669%
26	6.297	1634	1635	1639	rBV3	329	246	0.03%	0.003%
27	6.317	1639	1641	1643	rVV3	474	273	0.03%	0.004%
28	6.342	1647	1649	1651	rVB3	409	175	0.02%	0.002%
29	6.407	1667	1669	1671	rBV3	217	101	0.01%	0.001%
30	6.426	1671	1675	1677	rBV	229	196	0.02%	0.003%
31	6.487	1692	1694	1695	rBV	367	201	0.02%	0.003%
32	6.548	1710	1713	1714	rBV2	207	136	0.01%	0.002%
33	6.577	1721	1722	1724	rVB2	482	133	0.01%	0.002%
34	6.764	1778	1780	1782	rBV	364	204	0.02%	0.003%
35	6.780	1782	1785	1788	rVV2	306	179	0.02%	0.002%
36	6.799	1788	1791	1792	rBV	448	212	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031966.D
 Acq On : 31 Aug 2023 17:04
 Operator : SY/MD
 Sample : 04235-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.850	1806	1807	1808	rBV	337	117	0.01%	0.002%
38	6.918	1815	1828	1853	rBV	118885	228059	24.51%	3.072%
39	7.246	1919	1930	1964	rBV	416547	756938	81.34%	10.195%
40	7.497	2006	2008	2012	rBV3	418	346	0.04%	0.005%
41	7.558	2017	2027	2050	rBV	82341	151074	16.23%	2.035%
42	7.812	2104	2106	2107	rBV2	441	122	0.01%	0.002%
43	7.837	2113	2114	2116	rVB	633	136	0.01%	0.002%
44	7.854	2116	2119	2121	rVB3	444	246	0.03%	0.003%
45	7.870	2121	2124	2125	rBV	793	503	0.05%	0.007%
46	8.030	2164	2174	2212	rBV	212737	424462	45.61%	5.717%
47	8.516	2324	2325	2329	rVB	481	265	0.03%	0.004%
48	8.538	2329	2332	2334	rBV3	453	308	0.03%	0.004%
49	8.606	2350	2353	2355	rBV2	520	339	0.04%	0.005%
50	8.677	2372	2375	2379	rVB3	645	408	0.04%	0.005%
51	8.693	2379	2380	2383	rBV	306	167	0.02%	0.002%
52	8.731	2390	2392	2393	rBV2	519	152	0.02%	0.002%
53	8.789	2398	2410	2436	rBV	477294	795757	85.51%	10.718%
54	8.995	2471	2474	2476	rBV2	541	390	0.04%	0.005%
55	9.111	2508	2510	2514	rVB2	559	307	0.03%	0.004%
56	9.191	2533	2535	2539	rVB3	458	223	0.02%	0.003%
57	9.320	2573	2575	2576	rBV3	220	99	0.01%	0.001%
58	9.384	2593	2595	2598	rVB2	377	238	0.03%	0.003%
59	9.407	2598	2602	2603	rBV2	464	257	0.03%	0.003%
60	9.493	2624	2629	2632	rVB2	567	453	0.05%	0.006%
61	9.516	2632	2636	2640	rBV4	496	430	0.05%	0.006%
62	9.551	2644	2647	2648	rBV2	277	183	0.02%	0.002%
63	9.609	2662	2665	2669	rBV3	241	194	0.02%	0.003%
64	9.670	2681	2684	2688	rBV3	378	297	0.03%	0.004%
65	9.738	2701	2705	2709	rBV4	458	481	0.05%	0.006%
66	9.825	2730	2732	2733	rBV	262	137	0.01%	0.002%
67	9.924	2761	2763	2765	rBV	325	134	0.01%	0.002%
68	9.972	2776	2778	2779	rBV	387	162	0.02%	0.002%
69	10.072	2807	2809	2811	rVV2	449	228	0.02%	0.003%
70	10.098	2815	2817	2819	rBV	182	120	0.01%	0.002%
71	10.156	2824	2835	2859	rVV	253960	405047	43.53%	5.456%
72	10.313	2881	2884	2886	rBV2	555	387	0.04%	0.005%
73	10.381	2902	2905	2908	rBV	239	201	0.02%	0.003%
74	10.426	2918	2919	2922	rBV2	309	153	0.02%	0.002%
75	10.487	2932	2938	2941	rBV5	729	756	0.08%	0.010%
76	10.561	2958	2961	2963	rBV3	401	250	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
 Data File : VV031966.D
 Acq On : 31 Aug 2023 17:04
 Operator : SY/MD
 Sample : 04235-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.632	2981	2983	2985	rBV	351	168	0.02%	0.002%
78	10.667	2992	2994	2996	rBV	266	139	0.01%	0.002%
79	10.706	3005	3006	3009	rBV	379	135	0.01%	0.002%
80	10.741	3014	3017	3018	rBV	382	249	0.03%	0.003%
81	10.780	3026	3029	3031	rVB3	517	290	0.03%	0.004%
82	10.844	3047	3049	3051	rBV2	286	146	0.02%	0.002%
83	10.918	3069	3072	3073	rBV2	386	194	0.02%	0.003%
84	11.008	3096	3100	3101	rBV2	537	369	0.04%	0.005%
85	11.133	3137	3139	3140	rBV	362	146	0.02%	0.002%
86	11.188	3145	3156	3180	rVV	558431	863767	92.82%	11.634%
87	11.464	3241	3242	3246	rBV2	411	222	0.02%	0.003%
88	11.564	3261	3273	3297	rBV	437087	690887	74.24%	9.306%
89	11.915	3379	3382	3383	rBV	321	187	0.02%	0.003%
90	12.050	3420	3424	3425	rBV2	350	242	0.03%	0.003%
91	12.101	3437	3440	3441	rBV	491	221	0.02%	0.003%
92	12.130	3447	3449	3452	rBV2	663	453	0.05%	0.006%
93	12.239	3481	3483	3487	rBV	337	261	0.03%	0.004%
94	12.323	3507	3509	3513	rVB3	444	230	0.02%	0.003%
95	12.468	3551	3554	3555	rBV	476	212	0.02%	0.003%
96	12.603	3591	3596	3599	rBV4	796	717	0.08%	0.010%
97	13.304	3812	3814	3817	rBV4	463	282	0.03%	0.004%
98	13.349	3824	3828	3829	rBV2	511	307	0.03%	0.004%
99	13.435	3852	3855	3856	rBV	684	460	0.05%	0.006%
100	14.085	4055	4057	4061	rBV2	689	411	0.04%	0.006%




Sum of corrected areas: 7424258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031966.D
Acq On : 31 Aug 2023 17:04
Operator : SY/MD
Sample : 04235-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

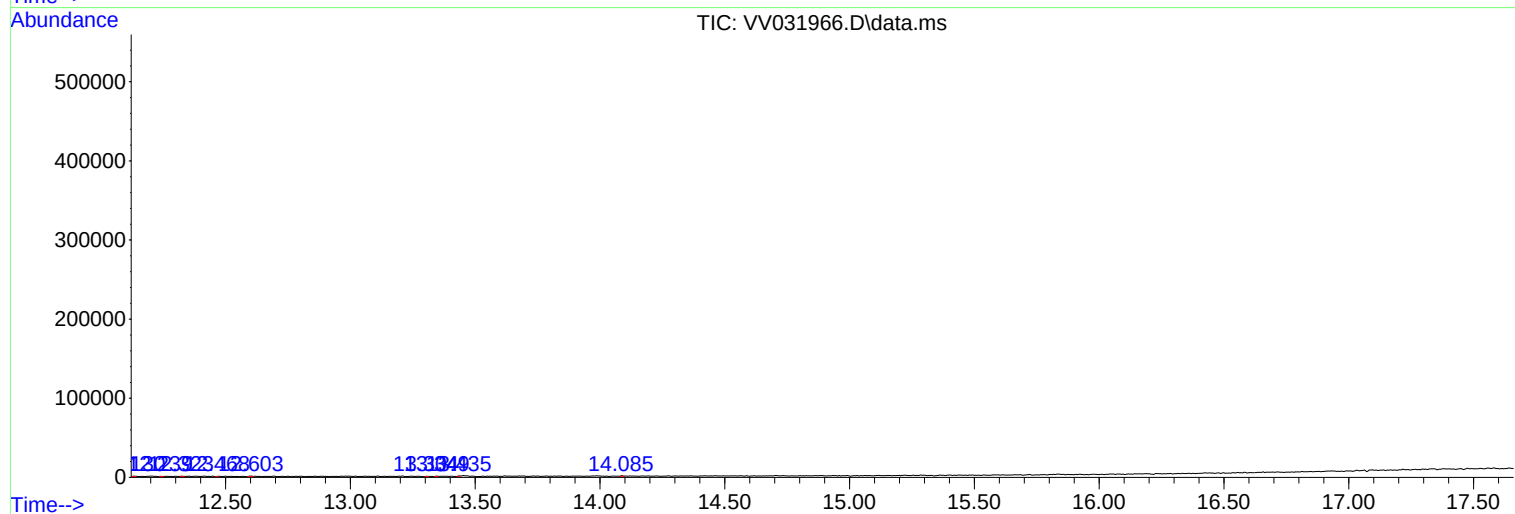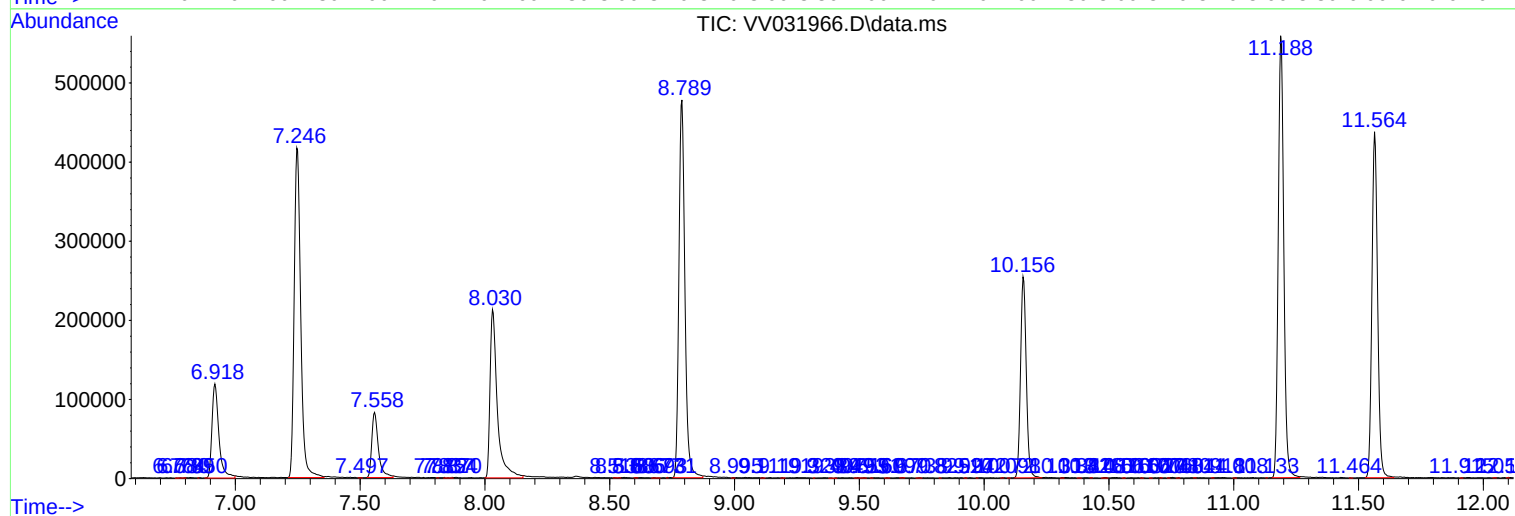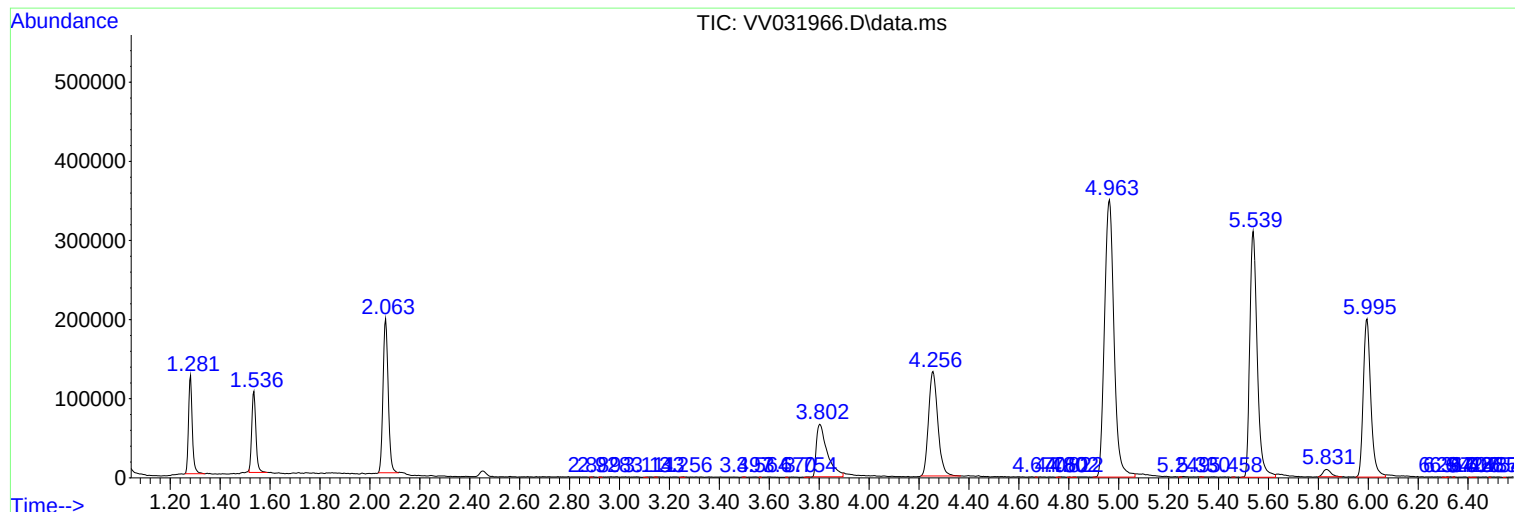

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031966.D
Acq On : 31 Aug 2023 17:04
Operator : SY/MD
Sample : 04235-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031966.D
Acq On : 31 Aug 2023 17:04
Operator : SY/MD
Sample : 04235-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc