


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083123\
Data File : VV031955.D
Acq On : 31 Aug 2023 10:55
Operator : SY/MD
Sample : BFB208
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB208

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Fri Sep 01 00:57:38 2023

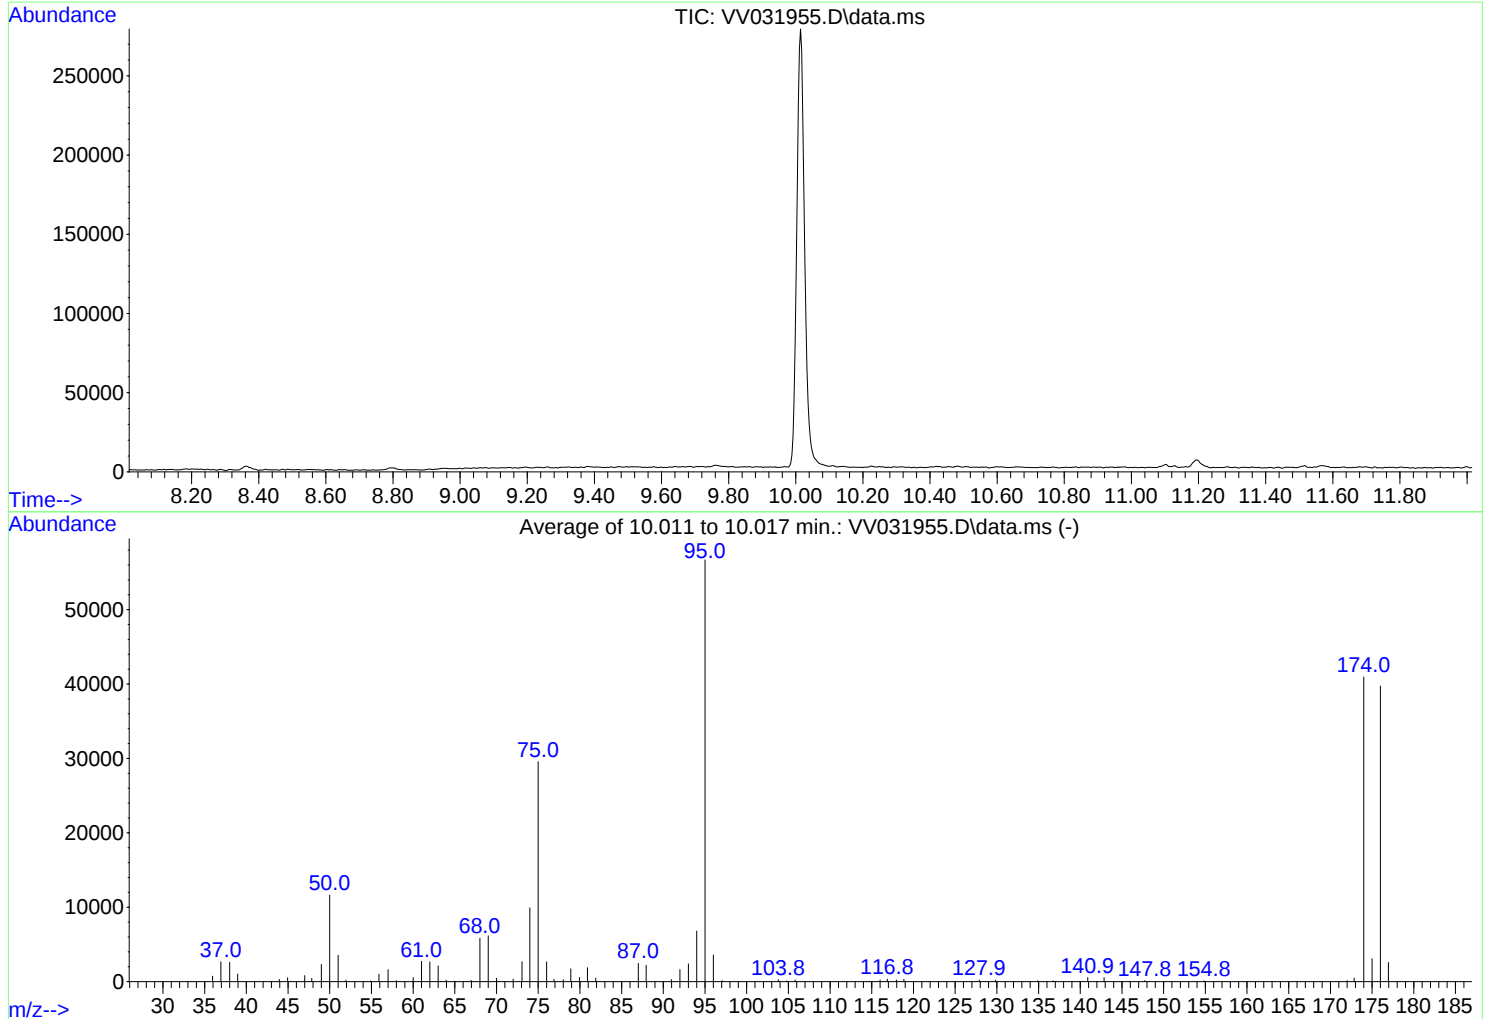

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	11643	PASS
75	95	30	80	52.2	29579	PASS
95	95	100	100	100.0	56691	PASS
96	95	5	9	6.3	3568	PASS
173	174	0.00	2	1.2	472	PASS
174	95	50	120	72.2	40936	PASS
175	174	5	9	7.5	3067	PASS
176	174	95	105	97.0	39712	PASS
177	176	5	10	6.5	2590	PASS

m/z	Abundance
35.90	1822.0
37.00	2862.0
38.00	3115.0
39.00	1184.0
39.90	197.0
41.00	191.0
42.80	179.0
44.00	787.0
44.90	513.0
47.00	819.0
47.90	446.0
49.00	2348.0
50.00	11977.0
51.00	3652.0
52.00	193.0
55.00	284.0
55.90	1057.0
57.00	1676.0
58.00	143.0
60.00	552.0
61.00	2807.0
62.00	2733.0
63.00	2157.0
63.90	198.0
65.00	106.0
66.90	182.0
68.00	5985.0
69.00	6409.0
70.00	480.0
72.00	360.0
73.00	2776.0
74.00	10222.0
75.00	30616.0
76.00	2749.0
76.90	418.0
78.00	265.0
78.90	1797.0
79.90	582.0
80.90	1946.0
81.90	482.0
87.00	2473.0
87.90	2268.0
90.90	287.0
92.00	1648.0
93.00	2429.0
94.00	7034.0
95.00	58640.0
96.00	3691.0
97.10	146.0
103.80	260.0
104.80	121.0
105.80	234.0
114.70	104.0
116.00	209.0
116.80	363.0
117.90	217.0
118.80	325.0
127.90	218.0
129.80	196.0
134.90	135.0
136.80	122.0
140.90	576.0
142.80	545.0
147.80	161.0
154.80	115.0
172.00	148.0
172.80	485.0
174.00	42352.0
175.00	3184.0
176.00	40984.0
176.90	2664.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	1050.0
36.90	152.0
38.00	427.0
38.90	115.0
39.90	236.0
41.00	120.0
42.00	133.0
43.00	142.0
43.90	496.0
54.80	187.0
77.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.90	1659.0
37.00	2989.0
38.00	3157.0
39.00	1221.0
40.00	224.0
41.00	201.0
42.80	166.0
44.00	791.0
45.00	559.0
47.00	793.0
47.80	399.0
49.00	2263.0
50.00	11715.0
51.00	3458.0
51.90	174.0
55.00	251.0
55.90	993.0
57.00	1650.0
58.00	144.0
60.00	557.0
61.00	2817.0
62.00	2592.0
63.00	2166.0
64.00	203.0
67.00	187.0
68.00	5817.0
69.00	6072.0
70.00	504.0
72.00	325.0
73.00	2718.0
74.00	9830.0
75.00	29280.0
76.00	2619.0
76.90	446.0
78.00	275.0
78.90	1694.0
79.90	560.0
80.90	1893.0
81.90	506.0
87.00	2428.0
88.00	2265.0
91.00	263.0
92.00	1665.0
93.00	2362.0
94.00	6868.0
95.00	56264.0
96.00	3692.0
97.00	150.0
103.80	238.0
104.80	108.0
105.80	195.0
116.00	208.0
116.90	322.0
117.90	223.0
118.90	346.0
127.90	217.0
130.00	187.0
134.90	114.0
136.70	106.0
140.90	531.0
142.90	530.0
147.70	149.0
154.80	110.0
172.00	152.0
172.80	428.0
174.00	39400.0
175.00	3059.0
176.00	38024.0
177.00	2587.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	1895.0
37.00	2609.0
38.00	2796.0
39.00	1028.0
39.90	194.0
41.00	179.0
42.90	174.0
44.00	787.0
44.90	453.0
47.00	828.0
47.90	444.0
49.00	2300.0
50.00	11237.0
51.00	3522.0
52.00	187.0
55.00	298.0
55.90	1010.0
57.00	1543.0
58.00	123.0
60.00	524.0
61.00	2546.0
62.00	2630.0
63.00	1993.0
63.90	169.0
65.00	110.0
66.90	181.0
68.00	5702.0
69.00	5962.0
70.00	402.0
72.00	338.0
73.10	2550.0
74.00	9666.0
75.00	28840.0
76.00	2562.0
76.90	394.0
78.00	238.0
78.90	1670.0
80.00	508.0
80.90	1778.0
81.90	446.0
87.00	2468.0
88.00	2114.0
90.90	261.0
92.00	1550.0
93.00	2360.0
94.00	6464.0
95.00	55168.0
96.00	3321.0
97.00	142.0
103.80	259.0
104.80	118.0
105.80	251.0
116.00	209.0
116.80	370.0
118.00	208.0
118.80	292.0
127.90	192.0
129.70	220.0
134.90	138.0
136.80	123.0
140.90	541.0
142.90	521.0
145.90	118.0
147.80	146.0
154.90	105.0
172.00	126.0
172.90	502.0
174.00	41056.0
175.00	2958.0
176.00	40128.0
176.90	2519.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208